

U.S. DEPARTMENT OF COMMERCE
National Technical Information Service

AD-A026 899

DEVELOPMENT OF HIGH PRESSURE LIQUID CHROMATOGRAPHIC
TECHNIQUES

NEW MEXICO UNIVERSITY

PREPARED FOR
AIR FORCE WEAPONS LABORATORY

MAY 1976

AFWL-TR-75-234

AFWL-TR-
75-234



DEVELOPMENT OF HIGH PRESSURE LIQUID CHROMATOGRAPHIC TECHNIQUES

Edward A. Walters

Civil Engineering Research Facility
University of New Mexico
Albuquerque, NM


May 1976

Final Report

Approved for public release; distribution unlimited.

AIR FORCE WEAPONS LABORATORY
Air Force Systems Command
Kirtland Air Force Base, NM 87117

REPRODUCED BY
NATIONAL TECHNICAL
INFORMATION SERVICE
U S DEPARTMENT OF COMMERCE
SPRINGFIELD, VA 22161



UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER AFWL-TR-75-234	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) DEVELOPMENT OF HIGH PRESSURE LIQUID CHROMATOGRAPHIC TECHNIQUES		5. TYPE OF REPORT & PERIOD COVERED Final Report
7. AUTHOR(s) Edward A. Walters		6. PERFORMING ORG. REPORT NUMBER CERF EE-3
9. PERFORMING ORGANIZATION NAME AND ADDRESS CERF University of New Mexico Albuquerque, New Mexico 87131		8. CONTRACT OR GRANT NUMBER(s) F29601-74-C-0030
11. CONTROLLING OFFICE NAME AND ADDRESS Air Force Weapons Laboratory (OL-AA, AFCEC) Kirtland AFB, NM 87117		10. PROGRAM ELEMENT PROJECT, TASK AREA & WORK UNIT NUMBERS 63723F 21034C44
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		12. REPORT DATE May 1976
		13. NUMBER OF PAGES 46
		15. SECURITY CLASS. (of this report) Unclassified
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) Approved for public release; distribution unlimited.		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from: Report)		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Liquid Chromatography Environmental Chemistry Detectors Water Pollutention Envionics High Pressure Liquid Chromatography		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) This is an interim report on a continuing study of the application of High Pressure Liquid Chromatographic (HPLC) techniques to water pollution problems. Reported herein are developmental data on three new detection systems; an ultra-sonic velocity detector, a beta-induced luminescence detector, and a specific solid-state silver-ion detector. Preliminary results of work on separations in natural waters and in sewage effluents using HPLC techniques and an extensive literature survey on HPLC are also included.		

This final report was prepared by the Civil Engineering Research Facility, University of New Mexico, Albuquerque, New Mexico under Contract F29601-74-C-0030, Job Order 21034C44 with the Air Force Weapons Laboratory, Kirtland Air Force Base, New Mexico. Major M. G. MacNaughton (OL-AA, AFCEC) was the Laboratory Project Officer-in-Charge.

When US Government drawings, specifications, or other data are used for any purpose other than a definitely related Government procurement operation, the Government thereby incurs no responsibility nor any obligation whatsoever, and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

This report has been reviewed by the Information Office (OI) and is releasable to the National Technical Information Service (NTIS). At NTIS, it will be available to the general public including foreign nations.


This technical report has been reviewed and is approved for publication.

Michael G. MacNaughton

MICHAEL G. MACNAUGHTON
Major, USAF, BSC
Project Officer

Kenneth R. Porter

KENNETH R. PORTER
Major, USAF, BSC
Commander, OL-AA, AFCEC

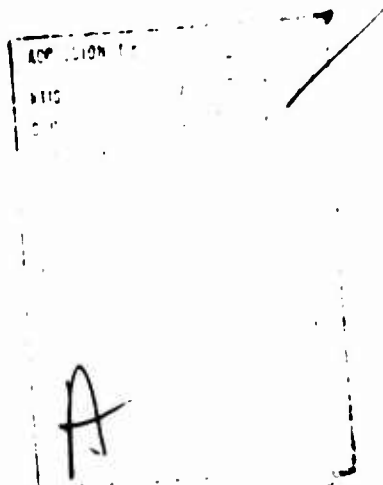

DO NOT RETURN THIS COPY. RETAIN OR DESTROY.

PREFACE

The original principal investigator, Dr. Nicholas E. Vanderborgh, left the University of New Mexico in January 1975 and supervision of the project was assumed by Dr. Edward A. Walters who has subsequently been responsible for the experimental direction, data analysis, interpretation, and presentation of results.

The electronics assistance of Fred Husher and the assistance and cooperation of Major Michael G. MacNaughton, Air Force Task Officer, are gratefully acknowledged.

CONTENTS

<u>Section</u>		<u>Page</u>
1	INTRODUCTION	5
2	LITERATURE SURVEY	7
3	DETECTOR DEVELOPMENT	8
	Ultrasonic Velocity	8
	Beta-Induced Luminescence	9
	Electrochemical Flowthrough	22
4	COLUMN AND CHROMATOGRAPHIC SYSTEM DEVELOPMENT	29
	APPENDIX: LITERATURE SURVEY LISTING	31

ILLUSTRATIONS

<u>Figure</u>		<u>Page</u>
1	Ultrasonic Velocity Detection System	10
2	Ultrasonic Velocity Detector	11
3	Electronics for Ultrasonic Velocity Detection System	12
4	Chromatogram Obtained with Prototype Beta-Induced Luminescence Detector	17
5	Tritium Foil Beta-Induced Luminescence Detector	18
6	Chromatograms Obtained with Second-Generation Beta-Induced Luminescence Detector	20
7	Electrochemical Flowthrough Detector	25
8	Solid-State Conduction System for Silver-Ion Detection	26
9	Electronics for Electrochemical Three-Electrode Detector	26
10	Electrochemical Three-Electrode Detection System	27
11	Chromatograms Obtained with Electrochemical Three-Electrode Detector	28
12	Chromatograms Obtained for EDTA Using Varian 4100 HPLC	30

TABLES

<u>Table</u>		<u>Page</u>
1	Response of Beta-Induced Luminescence Detection System to Nitrogen- and Halogen-Containing Organic Compounds	23

SECTION 1 INTRODUCTION

BACKGROUND

The Air Force as a result of its extensive maintenance activities discharges wastes which contain both metals and organics. Although total metals analysis is possible using atomic absorption and other instrumental and wet chemical techniques, the actual speciation of the compounds is unobtainable at present.

Knowledge concerning the types and concentrations of trace organics and metals in natural waters has become exceedingly more important in recent years as more data are gathered on their effect on humans, aquatic organisms, and plant life. Organics and organometallics even at the parts-per-billion level have been shown to exert a significant biotoxic and phytotoxic effect in fresh and marine waters.

The analysis of trace organics and metal organic complexes in the environment without disturbing the equilibrium which naturally exists is not possible with the present technology. All present techniques involve indirect measures of the speciation of the different elements. Extraction using organic solvents has been the most prevalent method of separating inorganic and organically bound metals into their separate fractions; however, this technique while applicable to gross differentiation of these two components does not give the actual species which exist in either fraction. Analysis by gas chromatography is useful only for those compounds which are volatile. Anodic stripping voltametry, an electrochemical technique, is also useful for determination of complexed metals which do not interfere with the electrodes and still gives limited data about complex solutions which contain organics and metals in both the free and complexed forms.

High Pressure Liquid Chromatography (HPLC) is a relatively new technique which has tremendous potential for analysis and identification of aqueous pollutants. Whereas with gas chromatography the compounds need to be volatile, with HPLC this is not necessary. Neither is it necessary to perform extractions of the

solutions and both metals and organics can be analyzed at the same time. Although HPLC is beginning to be used more extensively particularly in the analysis of drugs, to date there have been few reported uses of this technique in the identification and measurement of pollutants.

One of the most serious shortcomings of HPLC is the lack of detectors which would measure elution peaks from the liquid chromatograph with the same broad applicability as does the flame ionization detector in gas chromatography. The most common detectors available are the ultraviolet absorption and refractive index detectors. The ultraviolet detectors usually operate at the mercury line 253.7 nm or 280 nm and are useful only for those compounds which contain chromophores which absorb at these wavelengths. The refractive index detector lacks the sensitivity of the absorption detector and also exhibits a strong temperature dependence. What is needed in order to make HPLC a more generally applicable routine analysis are detectors which are general in their response to numerous elements or compounds.

OBJECTIVE

The objective of this research and development was to investigate HPLC techniques for the identification and measurement of organics and metals in natural waters. Specifically, this effort was concerned with the procedures, column materials, and detectors needed to establish reliable and accurate identification of trace organics and metal ions present in natural waters as a consequence of industrial discharges from Air Force installations.

SCOPE

The work reported herein deals with preliminary attempts to use HPLC for identification and quantification of metals and organics in aqueous systems, and the design and construction of three new potential detectors. Before beginning the laboratory work, a thorough survey was made of the literature on HPLC with particular attention directed toward applications to the identification of components of aqueous systems.

SECTION 2

LITERATURE SURVEY

A thorough search of all literature pertaining to HPLC was conducted. This was accomplished at the UNM library with the assistance of the Technology Application Center (NASA) which permitted a search through the Federal Documentation Center. The results of this search are included in appendix A. From this search it is quite evident that HPLC is growing rapidly, although the absence of documentation on the use of this technique to determine metal ion complexes is amazing. Apparently, many of these tasks are being performed by atomic absorption spectroscopy. However, atomic absorption simply gives a total metal concentration and offers no clues as to the chemical form of the metal before the determination. The literature search brought the realization that little material on HPLC appeared before 1972, and since that time much of the material of interest appeared in three journals; viz., *Journal of Chromatographic Science*, *Journal of Chromatography*, and *Analytical Chemistry*. Thus, much of the cited literature comes from these journals.

In addition a more general search on the subject of column chromatography was performed by the Technology Application Center. This search produced several thousand references, most of which deal with gas, not liquid, chromatography. These references cover all citations included in *Chemical Abstracts* during the period 1 January 1969 to 3 June 1974, as well as the abstracts. Because of bulk, this material is not included in this report, but it is available in the UNM General Library under the title *Column Chromatography*, LSS-100.

SECTION 3 DETECTOR DEVELOPMENT

ULTRASONIC VELOCITY

As an ultrasonic wave passes through a fluid medium, the phase, θ , is shifted according to the expression

$$\theta = 2\pi ft$$

where f is the frequency of the wave and t is the time required for the wave to pass through the fluid. This is related to the velocity, V , of the wave in the medium through

$$\theta = \frac{2\pi fr}{V}$$

where r is the distance traveled. The phase shift over this distance is

$$\frac{d\theta}{dr} = \frac{\omega}{V}$$

where $\omega = 2\pi f$. For a finite distance and a finite phase shift, the velocity can be calculated from

$$V = \omega \frac{\Delta r}{\Delta \theta}$$

If Δr is constant, the phase shift, $\Delta \theta$, gives the velocity of the wave. This velocity is highly dependent upon the type of fluid and thus may be used to detect changes in fluid composition. This principle has been employed in detectors for gas chromatography.

Unfortunately, however, phase shifts commonly occur when pulses traverse electronic circuits and so tedious calibrations are essential. Therefore, this research was oriented toward establishing the potential of a differential technique for velocity measurement by a phase shift which would obviate any electronic contributions by employing the same circuits for both channels.

Feasibility of a three-transducer, phase-shift concept was demonstrated and the work was described at *The Second Rocky Mountain Regional Meeting of the American Chemical Society* on 8 July, 1974 and in a paper (ref. 1). A detector with a large volume (approximately 20 mL) was employed in this feasibility test. However, a detector with a much smaller volume (approximately 5 mL) was constructed, and a detection system which would be compatible with an HPLC device and would also provide interfacing with a small computer was designed and constructed. In this detection system (fig. 1) the gated oscillator generates a continuous wave at 1 MHz. This wave is fed to one of two transmitters depending upon the state of the control logic. Three transducers are contained in the detector (fig. 2). The transmitters drive two of these transducers which are separated from the third, receiving transducer, by different fixed distances. The signal from the receiving transducer is amplified and beat against a local oscillator to lower the frequency to near 25 kHz. This signal is then sent to the phase meter and the phase shift is converted to a voltage which is read directly on a digital panel meter. Provisions are made for attaching a recorder or a computer. Schematics of the present system* are shown in figure 3.

BETA-INDUCED LUMINESCENCE

Again, a technique known to function as a detector in gas chromatographic systems was expanded upon in an attempt to construct an HPLC detector based on the concept of beta-ray-induced (quenched) luminescence. This detection system is based on the concept that as beta particles (products of the radioactive decay of tritium) slow down in passing through a medium, they transfer energy to the molecules encountered. Although beta rays from tritium are relatively soft (1.8 MeV), they have sufficient energy to cause excitation and/or ionization of many molecules. These excited molecules emit light as they decay to their ground states or as they recombine to form new products. This light can be detected with the customary photomultiplier system, and thus it can be used

-
1. Chen, Chuan, and Vanderborgh, Nicholas E., "A Three-Transducer Differential Phase-Shift Method for the Measurement of Ultrasonic Velocity in Liquids," *Review of Scientific Instruments*, (to be published).

*Recent changes will be indicated in the final report.

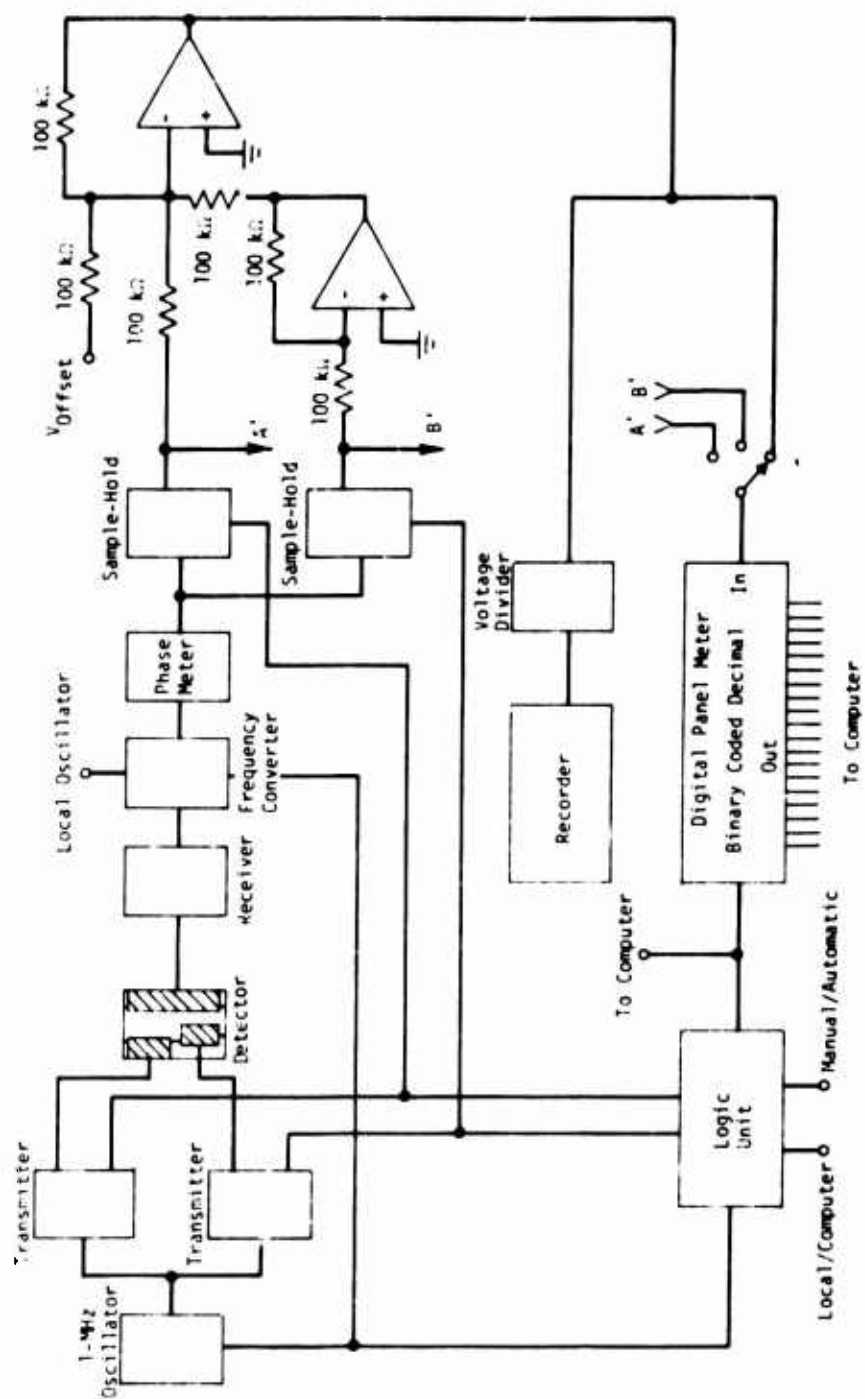


Figure 1. Ultrasonic Velocity Detection System

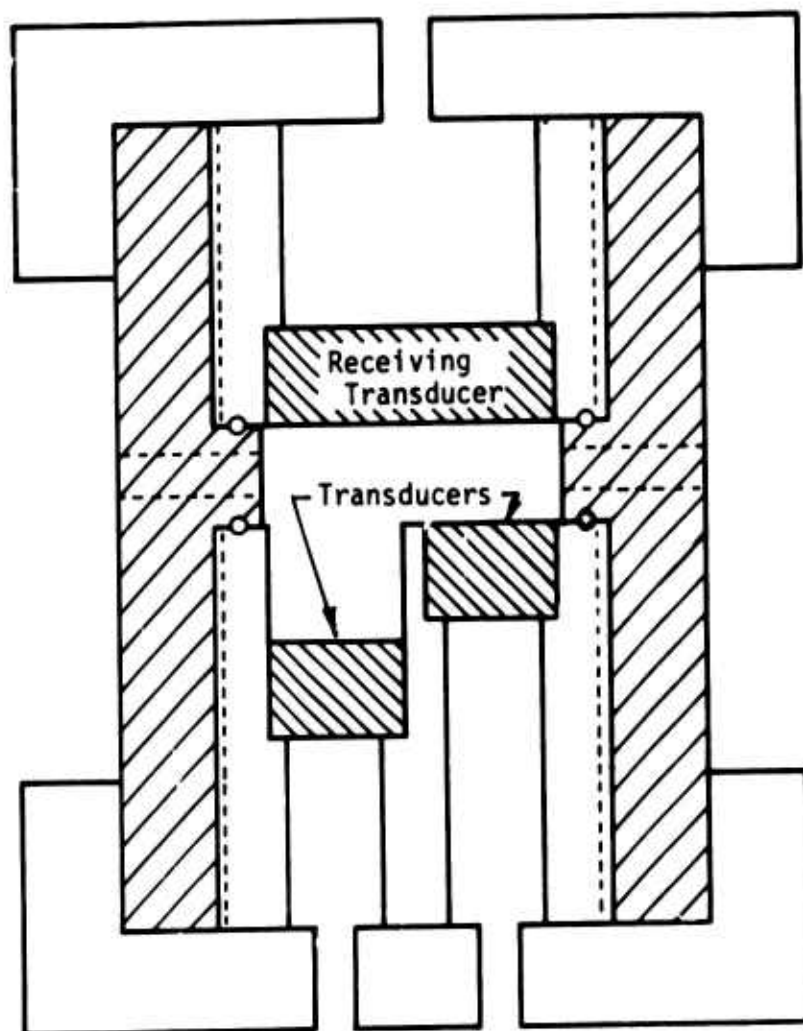


Figure 2. Ultrasonic Velocity Detector

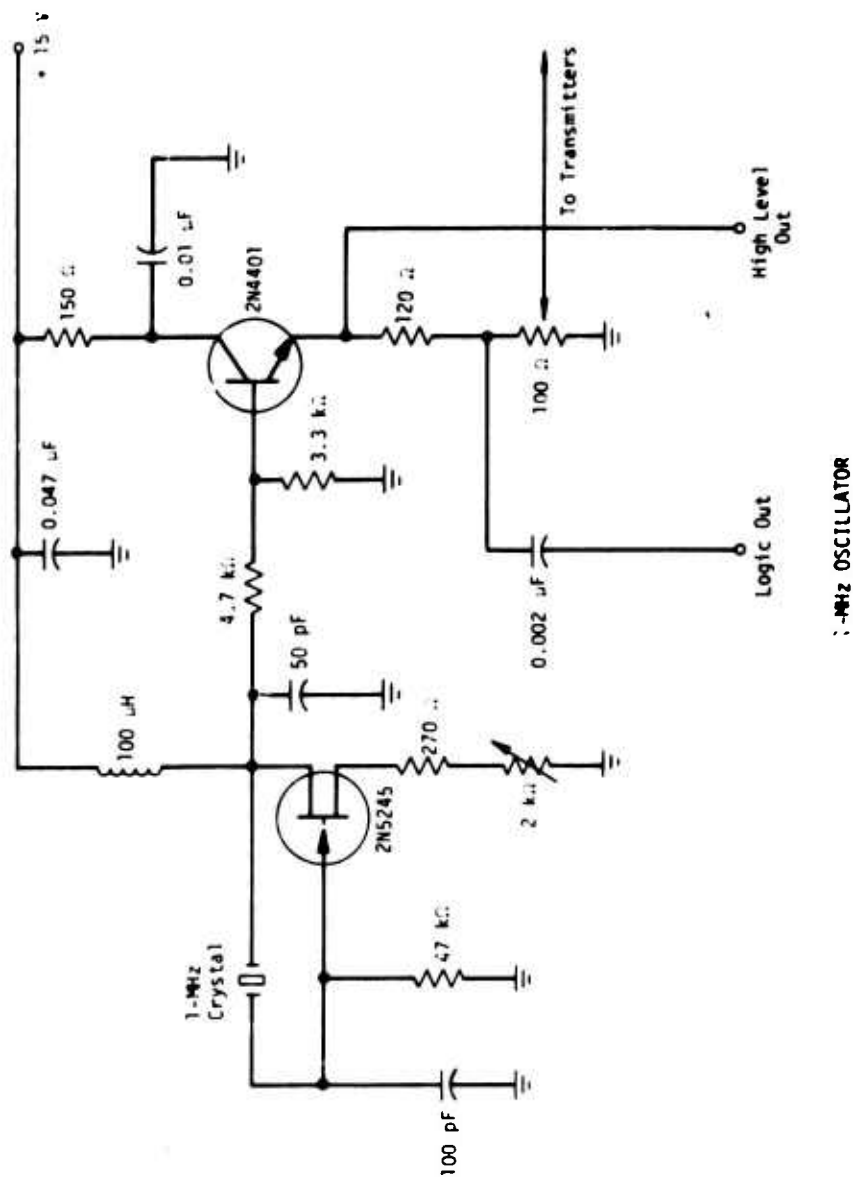


Figure 3. Electronics for Ultrasonic Velocity Detection System (1 of 4)

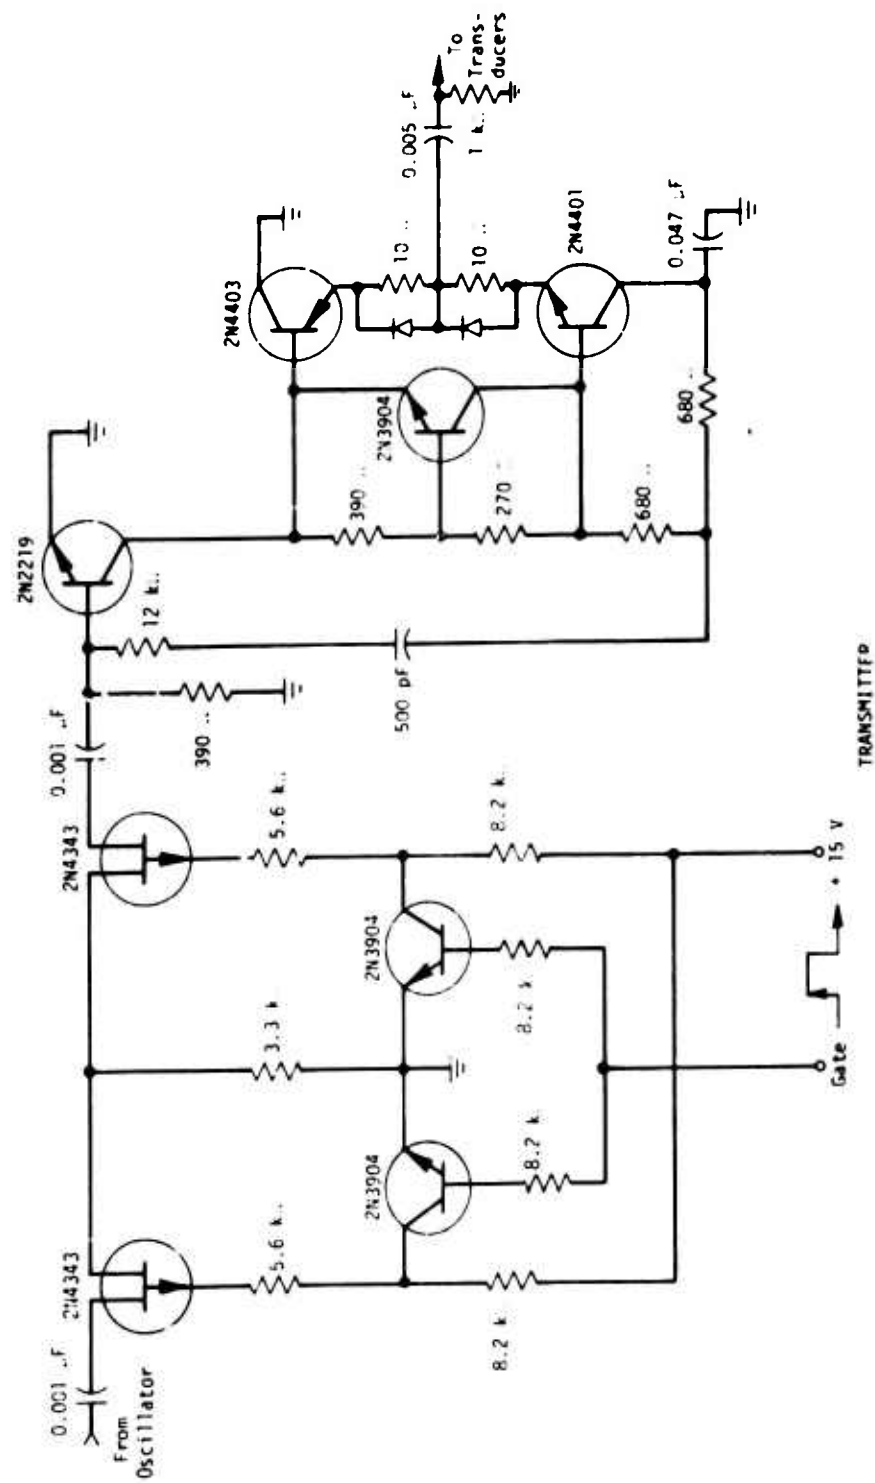


Figure 3. Electronics for Ultrasonic Velocity Detection System (2 of 4)

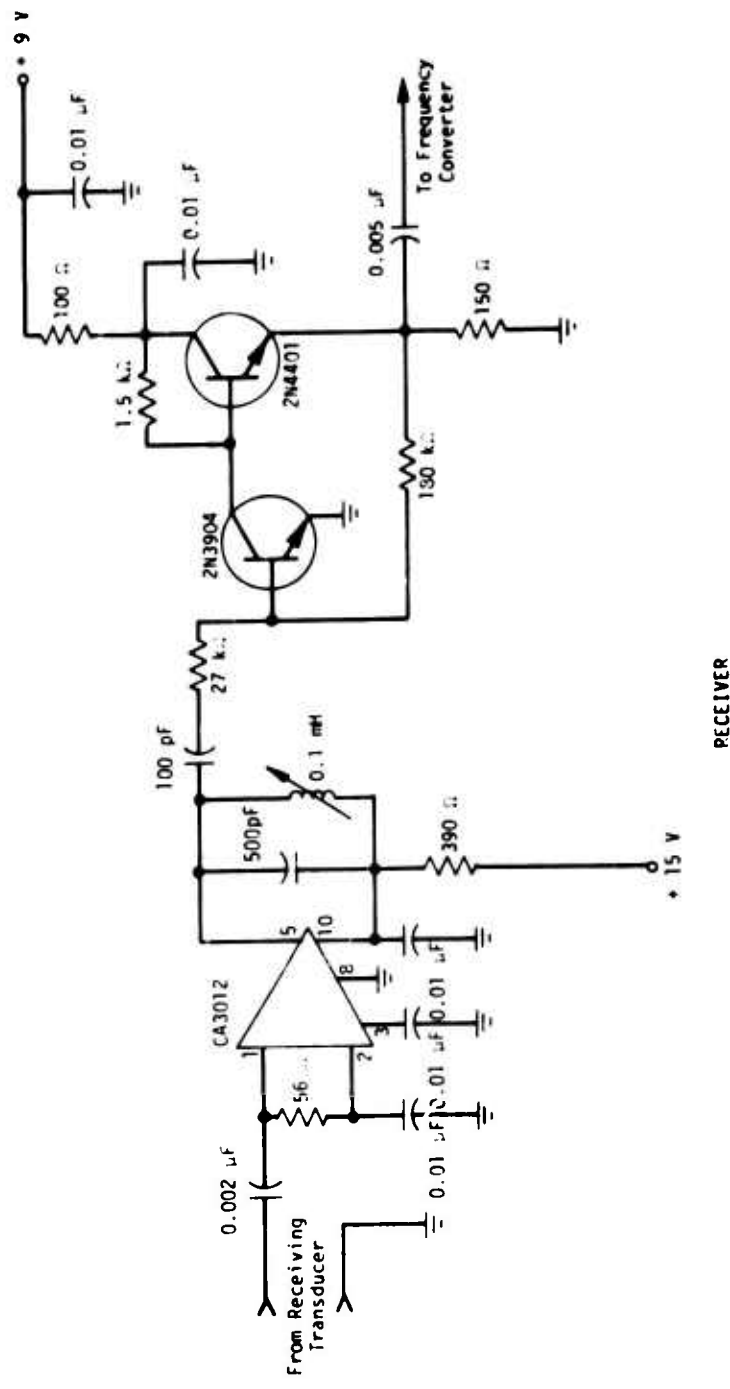


Figure 3. Electronics for Ultrasonic Velocity Detection System (3 of 4)

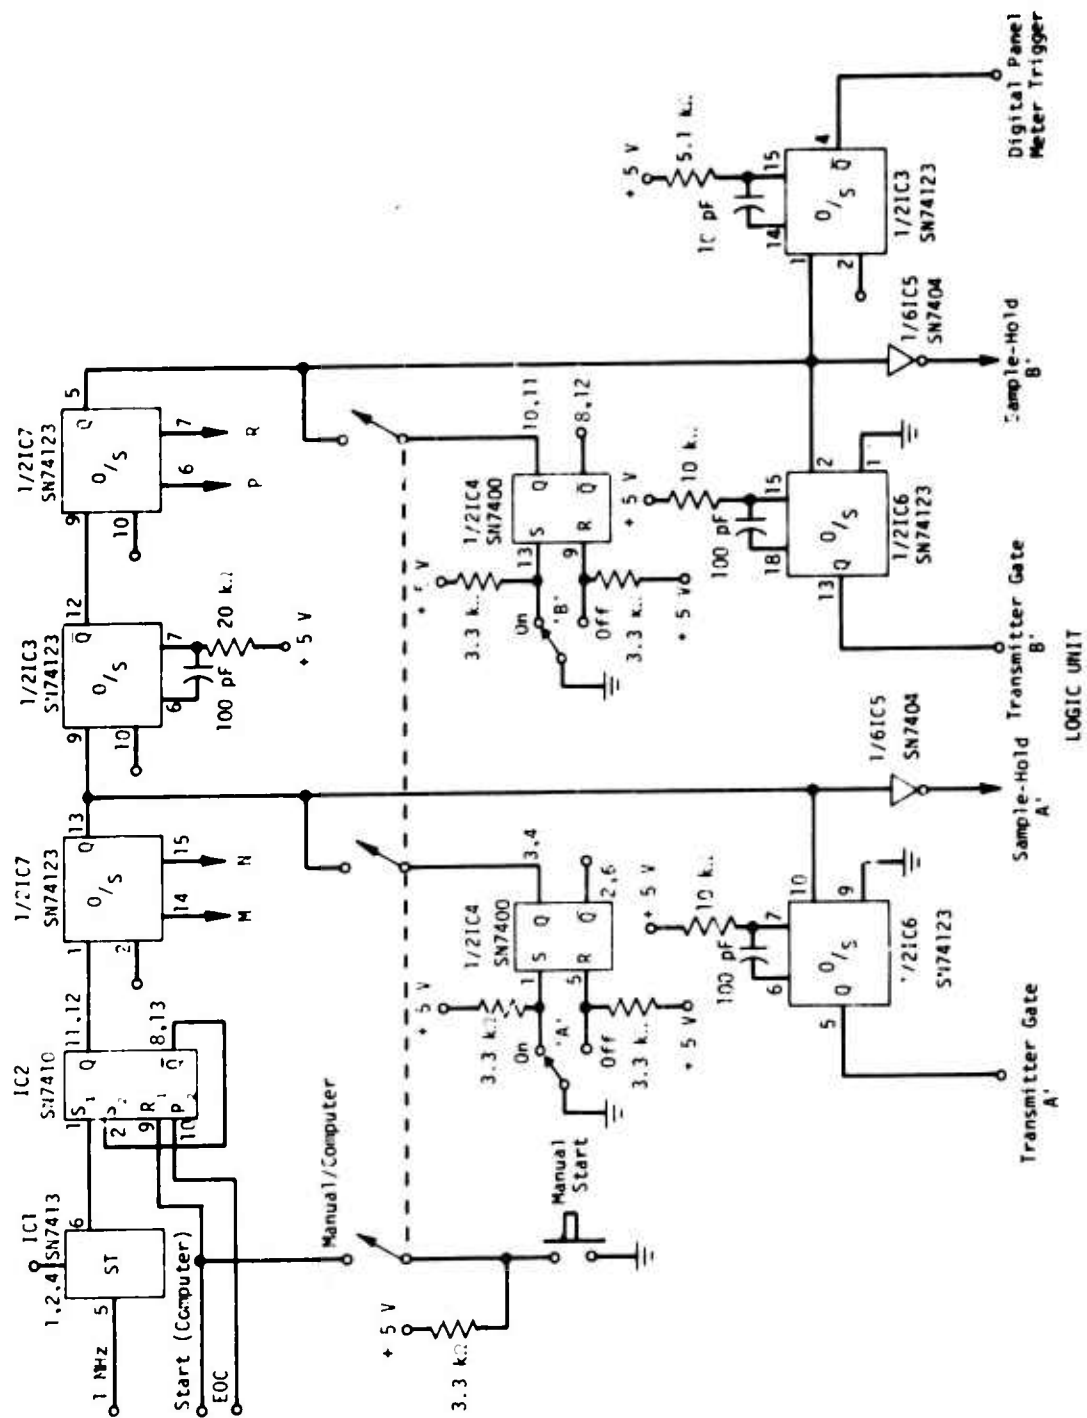


Figure 3. Electronics for Ultrasonic Velocity Detection System (4 of 4)

to determine the quantity of material in the path of the beta rays. In addition, the wavelength at which maximum fluorescence occurs is species dependent so that some distinction can be made between, say, solvent and solute.

Two detectors, a prototype and a second-generation model, were developed and tested. The prototype detector was designed to test the feasibility of the beta-induced luminescence concept in application to HPLC. This detector consists of a tritiated titanium foil over which the solvent/solute systems may pass. Luminescence is observed on an RCA 4440 photomultiplier tube whose output goes to a strip-chart recorder. The volume of the detector is relatively large ($> 100 \mu\text{l}$). The system was tested in the dynamic sense by placing the detector at the outlet end of a 1/8-in-diameter, 5-cm-long column packed with alumina. The column was driven by a low pressure pump (~ 40 psi).

The most satisfactory performance was obtained in the quenching mode. In this mode fluorescence from the solvent, which is typically an aromatic liquid such as toluene, is quenched by the solute. The most efficient quenching, and most sensitive response, was obtained with halogenated solutes. The response of this chromatographic detection system to $20 \mu\text{l}$ of chloroform (CH_3Cl) and $15 \mu\text{l}$ of carbon tetrachloride (CCl_4) is shown in figure 4.

Based on the foregoing preliminary experiments, a second-generation detector was designed and constructed. In designing this detector, the theoretical consideration that the intensity of the fluorescence is proportional to the activity of the radioactive source in disintegrations per second was taken into account. In addition, capture cross sections for beta particles by matter suggest that a path length of $25 \mu\text{m}$ should be sufficient to stop all the incident beta rays so that the flow thickness of the detector need not exceed this value. Thus the resulting detector has the desired small volume of $4 \mu\text{l}$. This detector (fig. 5) consists of a head which houses the radioactive source and is covered by a cap through which luminescence is viewed. The sample flows transversely across the viewing region and the path length is controlled by spacers inserted between the head and the cap. All of the metal parts are stainless steel except the spacer which is brass shim stock cut to the appropriate shape; the window is quartz.


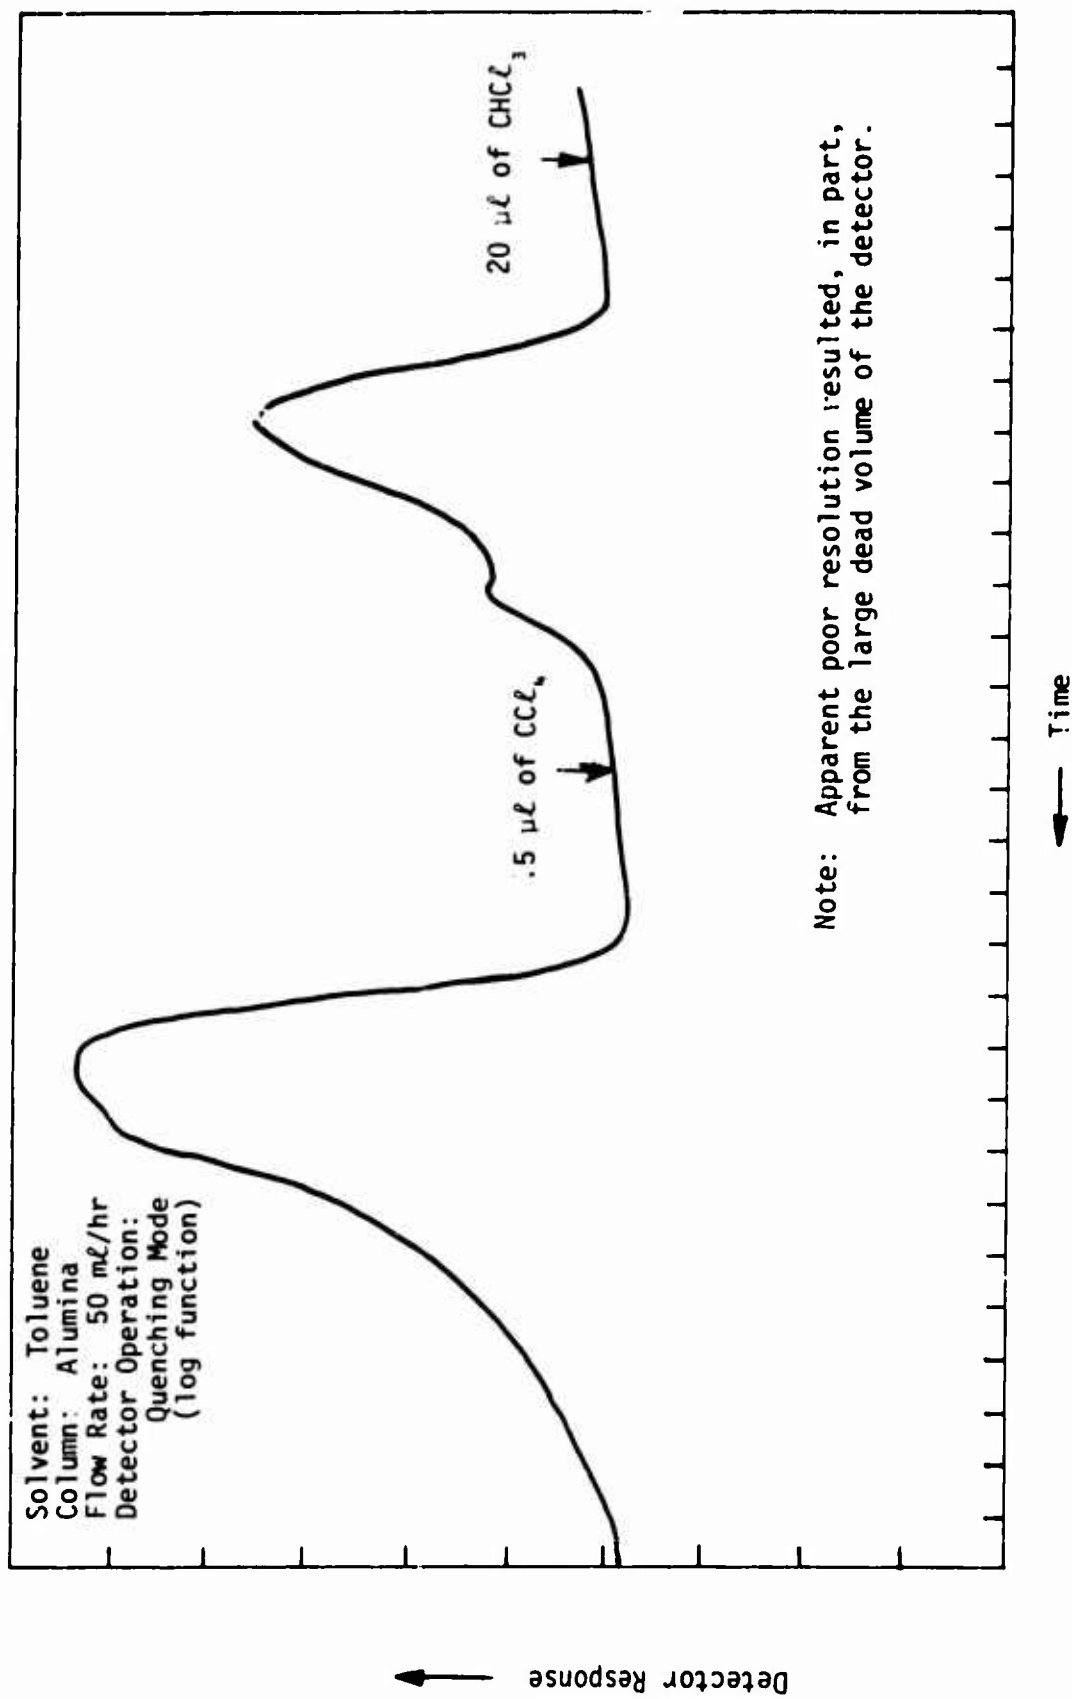


Figure 4. Chromatogram Obtained with Prototype Beta-Induced Luminescence Detector

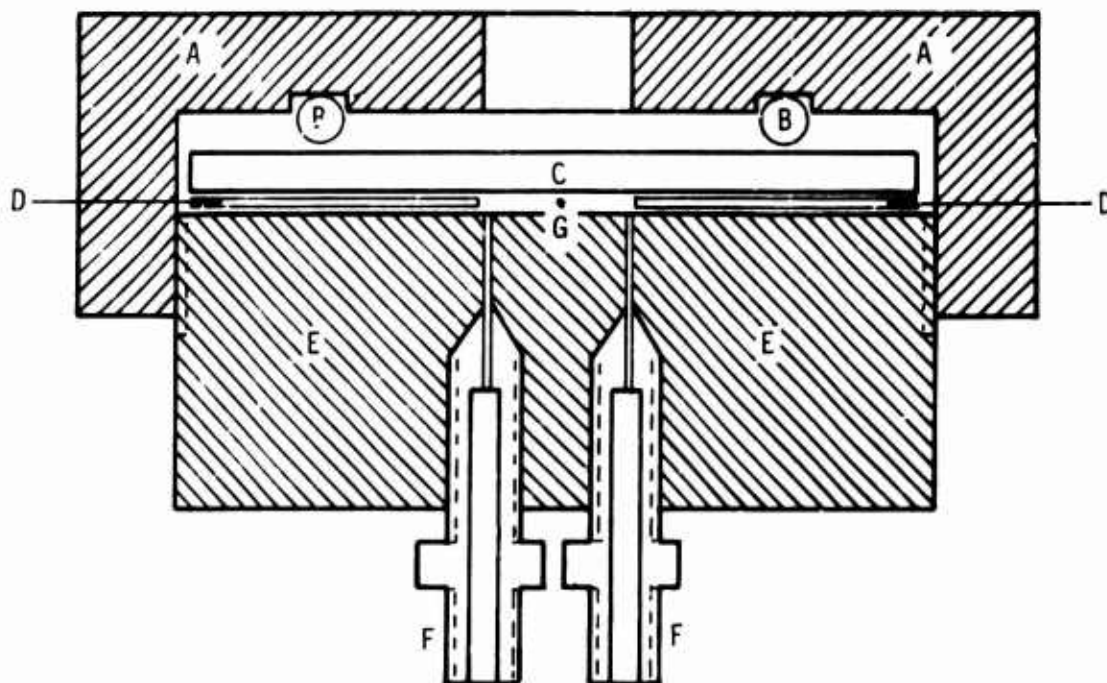

- A. Stainless Steel Cap
- B. Rubber O-Ring
- C. Quartz Lens
- D. 50- μ m Brass Spacer
- E. Stainless Steel Block
- F. Low Dead Volume Swagelock Fittings
- G. 1-cm-Diameter Circle with 1- μ m-Thick Layer of Titanium Vapor Deposited for Lattice to Hold 300 mCu of Tritium

Figure 5. Tritium Foil Beta-Induced Luminescence Detector

Tritiation of the detector head was carried out by Dr. John Crawford of Sandia Laboratories. On the surface of the head, a 1-cm-diameter, 1- μ m-thick film of titanium was applied using a sputtering technique. This layer was tritiated to an activity of 300 mCu using a vacuum-alloying procedure. The block as received was rather extensively contaminated with tritium; it was carefully decontaminated under the supervision of the UNM Radiological Safety Officer. The assembled detector was satisfactory as far as radioactivity was concerned, and the typical organic solvents flowing through the detector did not leach any radioactive materials.

The light-sensitive device initially employed was an RCA 4440 photomultiplier tube (same as in the prototype experiments). However, because of the short path length (25 μ m), the emitted photons were chiefly in the ultraviolet region, a region to which the RCA 4440 photomultiplier does not respond. Therefore, this tube was replaced with a 1P28 tube - a tube which responds well down into the ultraviolet region. A much more satisfactory detector was thus obtained.

As with the prototype detector, the quenching mode was the most useful. In fact, dynamic tests were made to monitor the quenched fluorescence of a standard scintillator solution. The solution was prepared by dissolving 5g of PPO and 0.3g of dimethyl POPOP in 1 l of xylene. This was used as the solvent into which 1- μ l samples of solutes were injected. A 5-cm glass column packed with beads of Poropak P was used.

A variety of test compounds was injected into the system ahead of the Poropak P column, and the detector response was recorded (fig. 6). These tests were made at a flow rate of approximately 2 ml/min so that the detector volume was changed about once every 0.3 sec.

Several observations can be made from these results. First, halogenated compounds give a significant response; that is, halogenated substrates are good quenchers. With the still reasonably crude second-generation detection system, it is possible to obtain a large response with 1- μ g samples. Improvements in the detector should increase the sensitivity of the system by about two orders of magnitude. This means that the detector used in the luminescence quenching mode should make a good detector for low levels of the halogenated

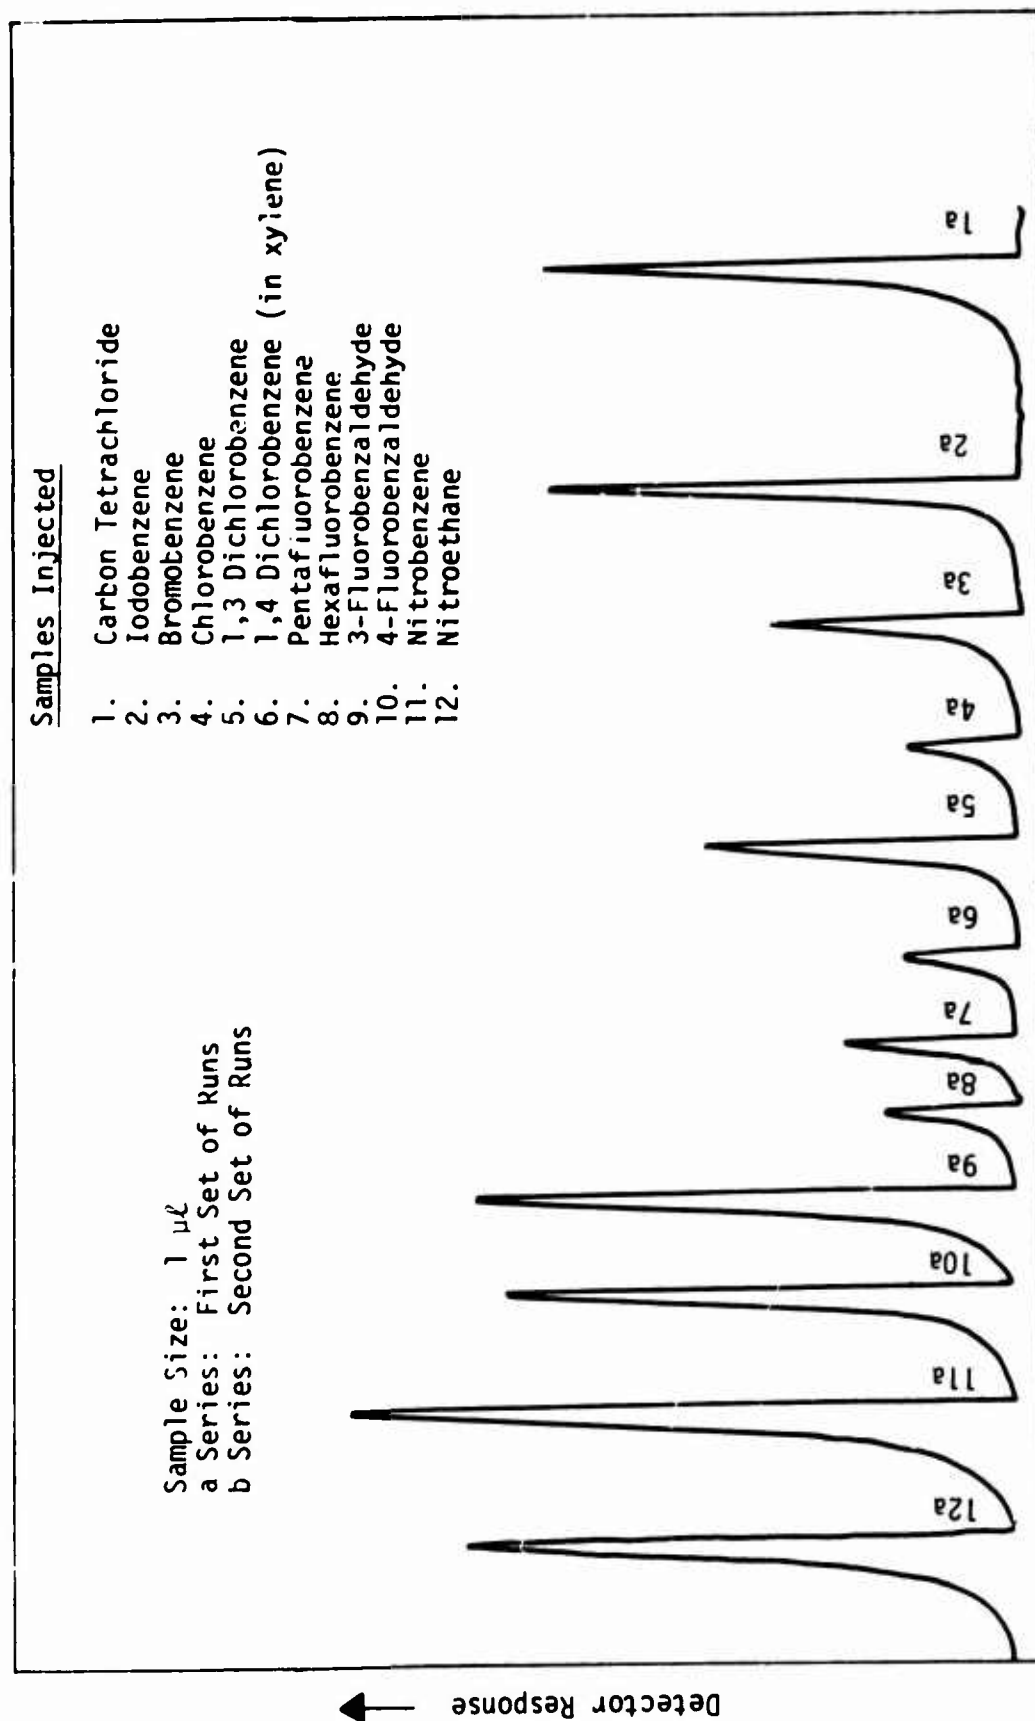


Figure 6. Chromatograms Obtained with Second-Generation Beta-Induced Luminescence Detector (1 of 2)

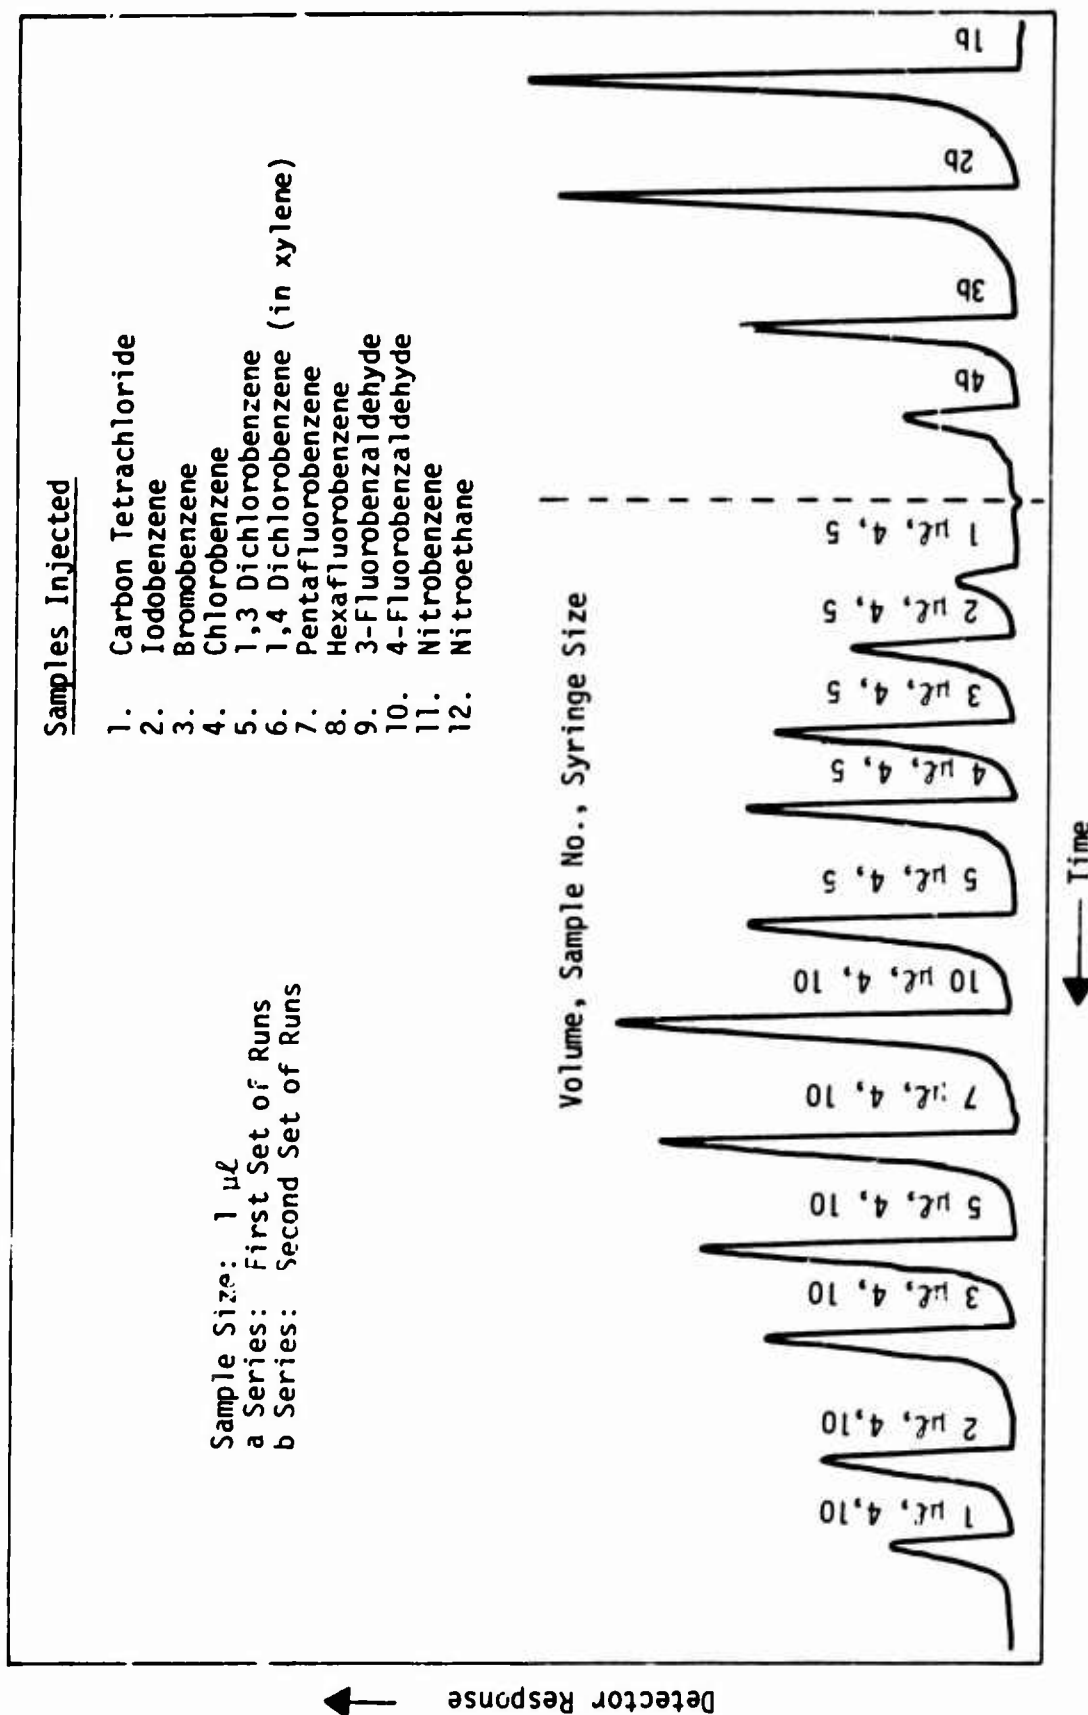


Figure 6. Chromatograms Obtained with Second-Generation Beta-Induced Luminescence Detector (2 of 2)

pesticides. Second, the response is dependent upon the chemical species employed. The response of a number of compounds relative to nitrobenzene is given in table I. Although this means that quantification of the chromatograms requires determination of quenching factors for each substrate, it also provides a somewhat more straightforward means of qualitative identification. Third, compounds containing nitro groups are the strongest quenchers; they are typically a factor of two more effective than even the halogenated hydrocarbons. Again, good response was found in all cases at or below the 1- μ g level. This is significant because, when compared to the detector volume, it is evident that solutes which fill far less than a single detector volume can be detected.

It seems reasonable that increasing the path length, while keeping the volume constant, will permit experimentation in both the luminescence and luminescence quenching modes. However, altering the path length of this detector is exceedingly inconvenient, so a third-generation detector with a variable path length is being designed.

ELECTROCHEMICAL FLOWTHROUGH

The goal in the electrochemical aspect of this project was to explore both general and specific electrochemical flowthrough detectors for metal ions. As a result of some very interesting pilot studies involving a solid-state, silver-ion conductor, work was concentrated on a specific silver-ion detector. A compound with the formula $\text{Ag}_6\text{I}_4\text{WO}_{12}$ is an ionic conductor at room temperature. Conductivity is due exclusively to the migration of Ag^+ through the crystal lattice. Efforts were directed toward developing a specific silver-ion electrochemical detector based on this observation. Various approaches were used.

Silver iodide-tungstate was prepared in the following manner. Silver tungstate was prepared by precipitation from equimolar solutions of sodium tungsten oxide (Na_2WO_4) and silver nitrate (AgNO_3). The precipitate was filtered, washed, and dried in a vacuum at 120°C. Silver iodide (AgI) was prepared and dried in the same way. Stoichiometric amounts of silver tungsten oxide (Ag_2WO_4) and AgI were carefully blended and annealed in a dark furnace at 400°C. The fused material was then reduced to a powder by grinding.

Table 1. Response of Beta-Induced Luminescence Detection System to Nitrogen- and Halogen-Containing Organic Compounds

Liquid Sample	$\left[\frac{\text{Relative Height Intensity (sample)}}{\text{Intensity (nitrobenzene)}} \right]$
nitrobenzene	1.00
m-nitrotoluene	0.98
o-nitrobenzene	0.96
o-fluorobenzaldehyde	0.75
nitroethane	0.73
p-fluorobenzaldehyde	0.67
iodobenzene	0.60
o-dichlorobenzene	0.40
2-chloro-6-methoxypyridine	0.38
quinoline	0.38
bromobenzene	0.37
pentafluorobenzene	0.23
chlorobenzene	0.19
4-picoline	0.19
hexafluorene	0.18
p-dichlorobenzene	0.13
N-methylpiperazine	-0.03


Note: All samples consisted of 4 μl of the liquid; retention time ranged between 8 and 12 min; and peaks were broad due to slow elution.

In one configuration, pellets of $\text{Ag}_6\text{I}_4\text{WO}_4$ were prepared by compressing the powder in a press to 20,000 psi. A pellet was incorporated in the detector as shown in figure 7. The saturated calomel electrode was protected by a saturated potassium nitrate (KNO_3) second junction. Maintaining a constant reference solution and varying silver-ion activity in the test solutions under potentiometric conditions resulted in a Nernstian response with a dynamic range of more than four orders of magnitude. When used to measure potential changes caused by the flow of trace amounts of Ag^+ past the detecting crystal, it gave a sub-micromolar response.

A second concept currently under investigation is the use of a $\text{Ag}_6\text{I}_4\text{WO}_4$ pellet as a membrane capable of transporting only Ag^+ (fig. 8). The idea is to impose a potential upon the electrode in such a way that conduction of Ag^+ across the membrane is impossible unless Ag^+ occurs on the test side, at which point a large drop in resistance across the membrane occurs. This drop, detected by standard instrumentation, measures the Ag^+ present in the flowing stream. The electronics for this system are shown in figure 9. The potential is set up across the detector, and the current flowing when Ag^+ is present on the test side is measured as a voltage at the output of one of the 118J operational amplifiers.


Finally, a three-electrode system was constructed. The detector is a working electrode held at a specific, but variable, potential in order to respond to electroactive components as they pass by. The conventional potentiostatic system is used with an auxiliary electrode and a calomel reference electrode. The detector and the amperometric and potentiometric mode circuits are shown in figure 10. A preliminary specific silver-ion working electrode was constructed by mixing $\text{Ag}_6\text{I}_4\text{WO}_4$ powder in just enough Duco cement to thoroughly wet the powder, dipping a silver wire into the mixture, drying the electrode, and repeating the process until an even, thin layer of electrode material was built up.

Tests made with both static and flowing systems confirmed a high response to Ag^+ and no response to a large number of other substances including CH_3OH , Cr^{+3} , Na^+ , K^+ , and NO_3^- . Chromatograms of the Ag^+ response are shown in figure 11. Sample sizes varied from 1 to 4 μl of 5×10^{-4} M AgNO_3 , or approximately 1 μg . Recorder sensitivity was not at its highest, and the detecting circuit was rather crudely breadboarded. However, improvements in construction should increase the sensitivity, perhaps into the low nanogram region.

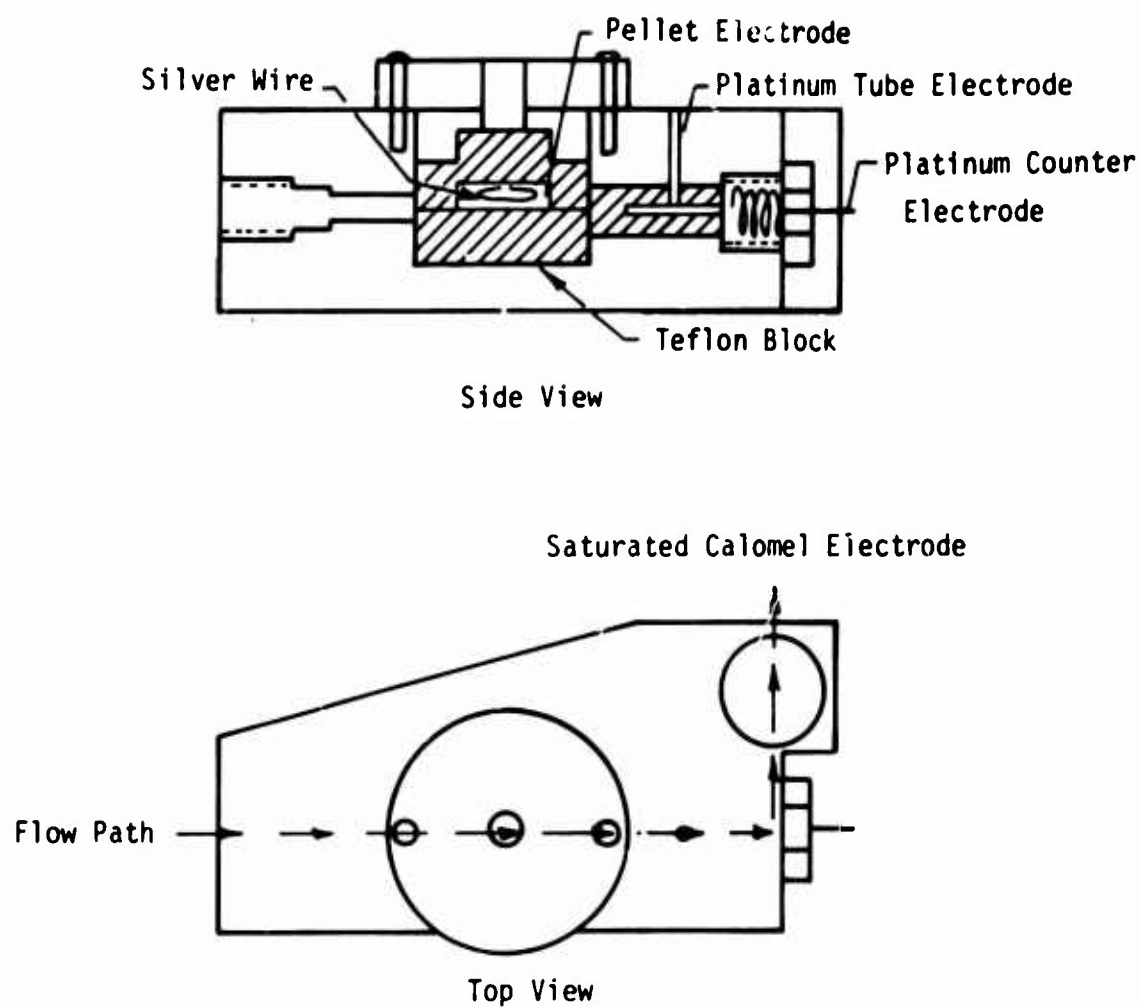

Note: This device permits simultaneous solid-electrolyte and voltammetric detection.
(Initial studies were on the silver ion.)

Figure 7. Electrochemical Flowthrough Detector

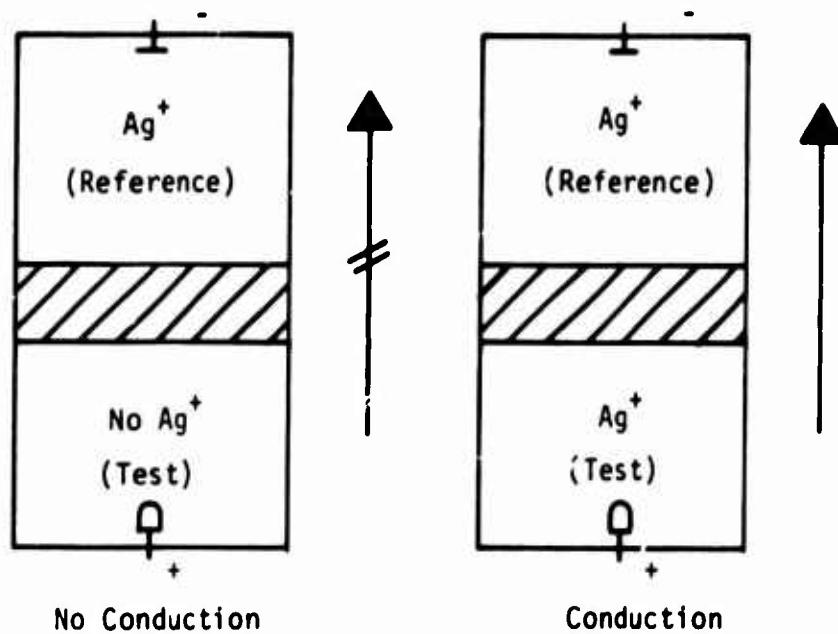

Crystal of Room-Temperature, Ionic-Conducting Material

Figure 8. Solid-State Conduction System for Silver-Ion Detection

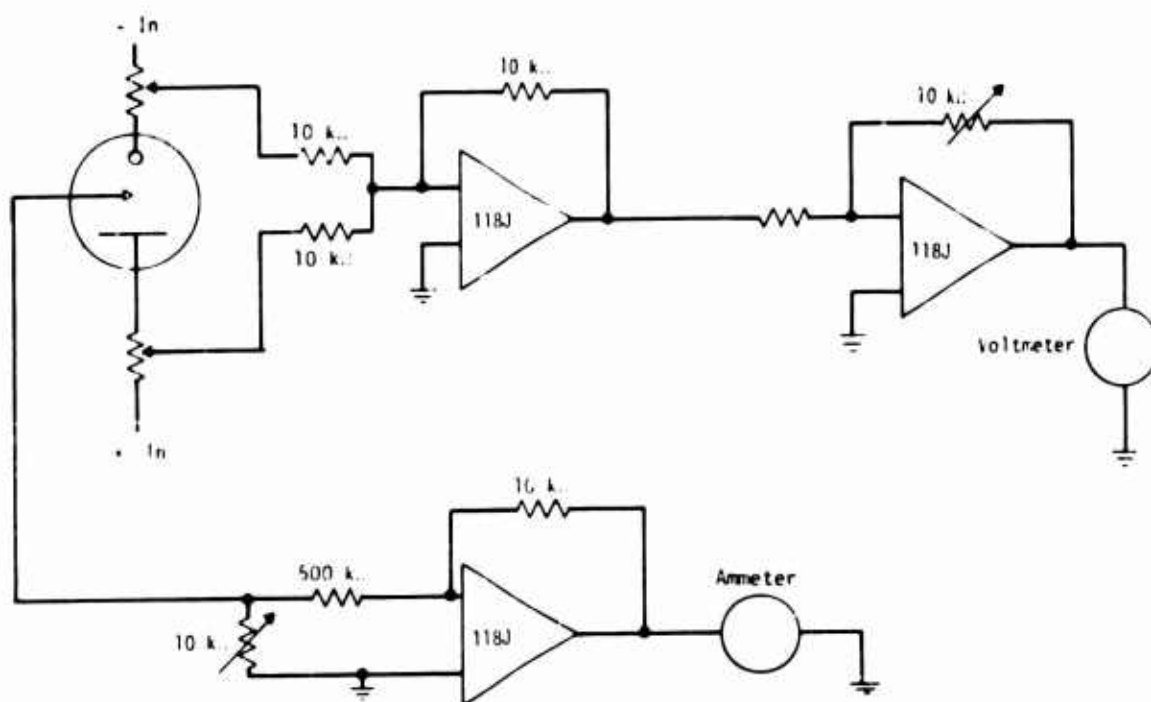


Figure 9. Electronics for Electrochemical Three-Electrode Detector

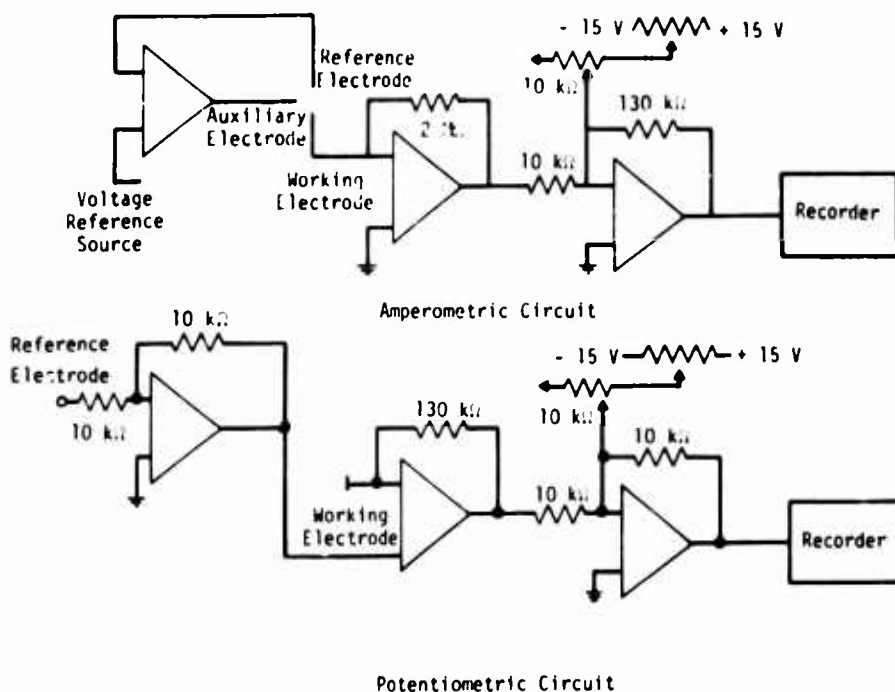
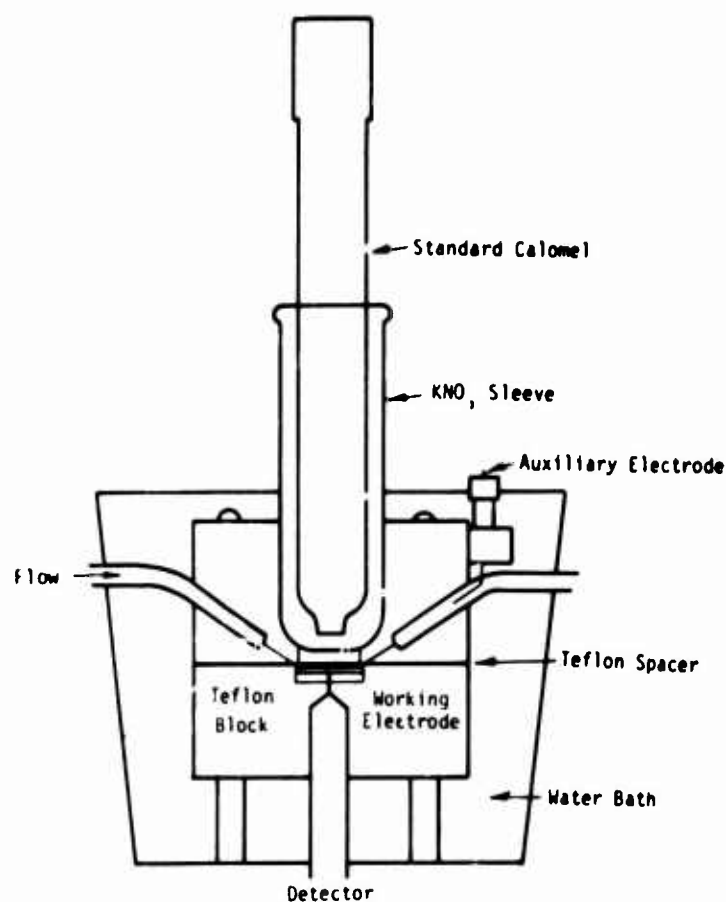


Figure 10. Electrochemical Three-Electrode Detection System

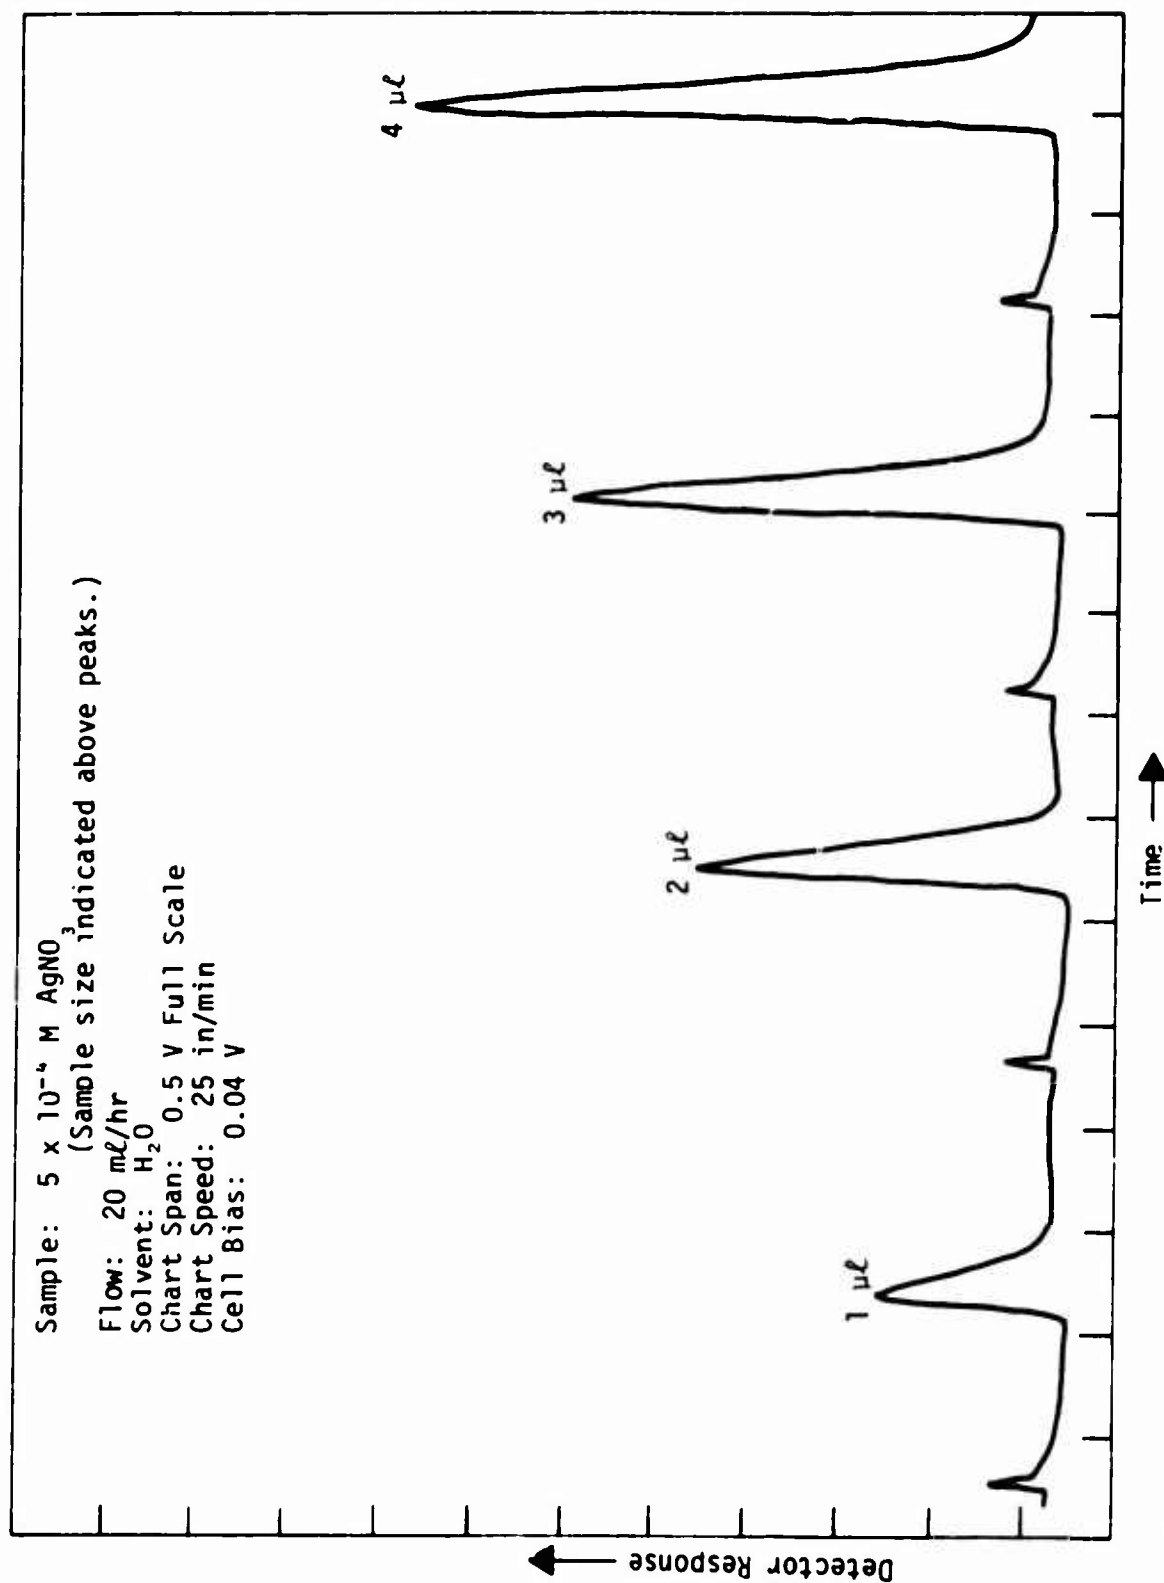


Figure 11. Chromatograms Obtained with Electrochemical Three-Electrode Detector

SECTION 4

COLUMN AND CHROMATOGRAPHIC SYSTEM DEVELOPMENT

A Varian 4100 HPLC system was transferred from AFWL and installed in the CERF laboratory. This system was tested and calibrated with nitroanilines in aqueous methanol solutions (70 pct by volume methanol) on a silica column.

Some preliminary experiments directed toward exploring the potential for separations of metal ions by the HPLC technique were performed. The concept being tested is the formation of complexes with complexing agents such as EDTA which have strong absorbances in the ultraviolet region so that the appearance of metal-complexed EDTA can be ascertained with the standard ultraviolet absorbance detector as it emerges from a liquid chromatographic column. Experiments with 0.75 μl of 0.01 M EDTA injected into the column and chromatographed gave the response shown in figure 12. This figure shows the response to 7.5×10^{-9} moles of EDTA. The peak could be attenuated by a factor of 50 and still be discernible over the baseline. Next, solutions of AgNO_3 in an excess of EDTA were chromatographed; a clear separation of the silver-EDTA complex from EDTA was observed. This points to the potential of using this method to separate metal ions in the conventional HPLC system.

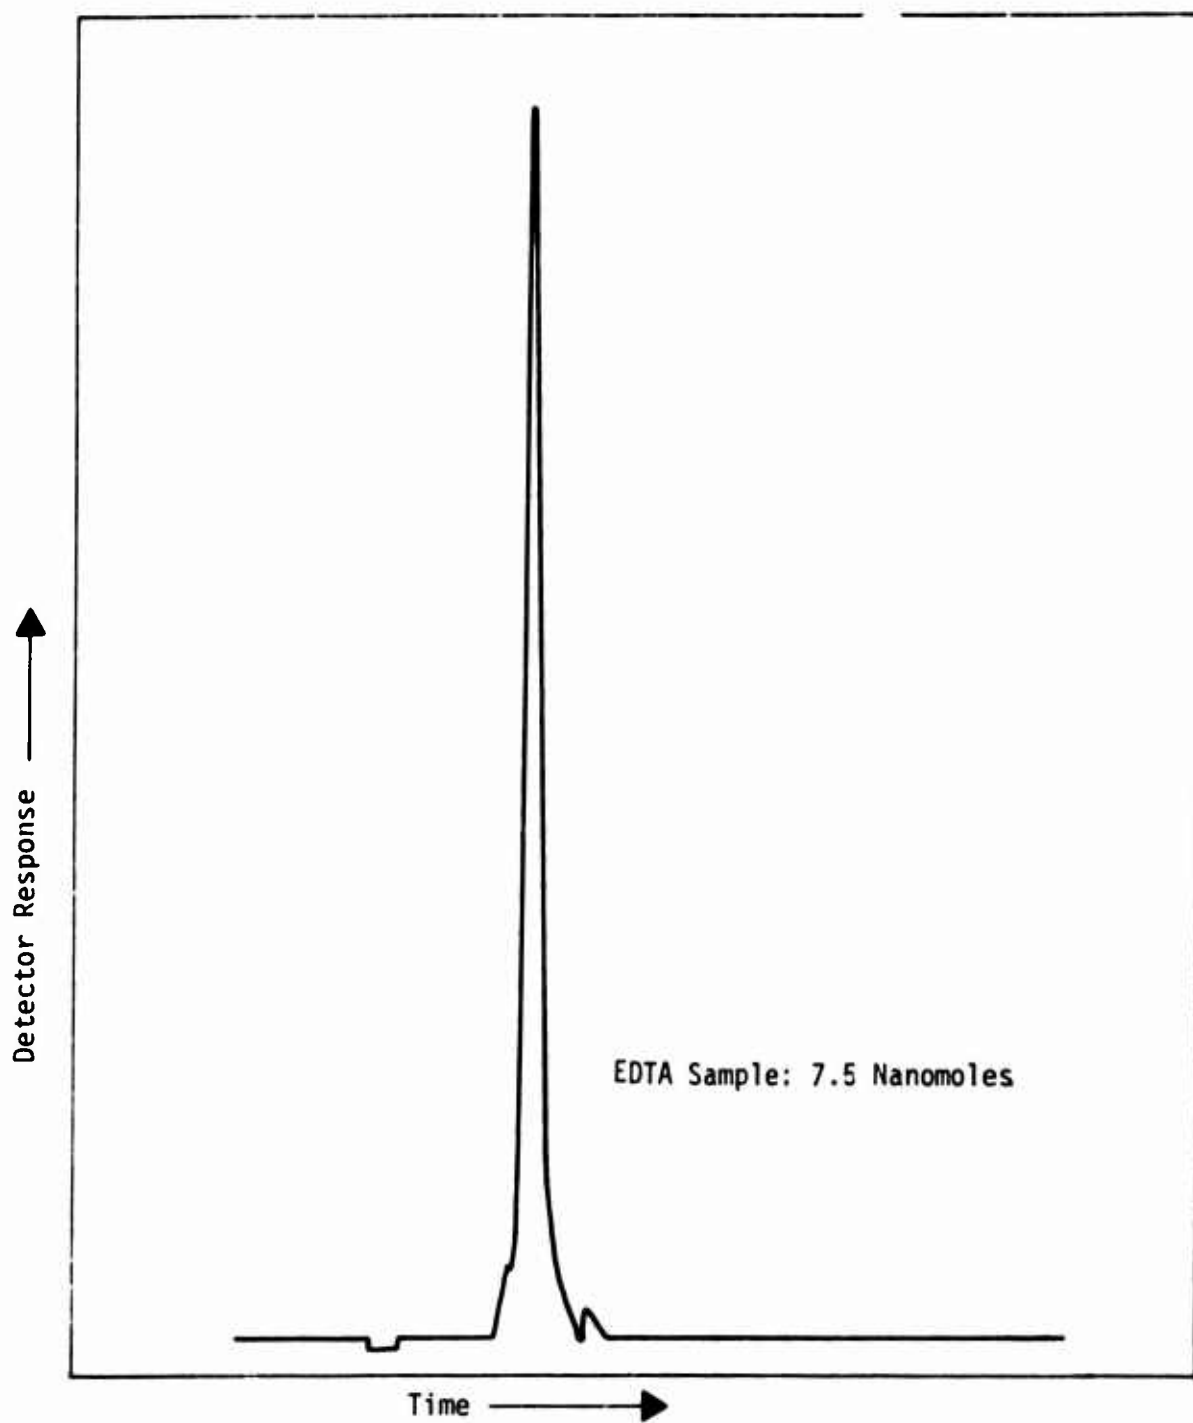


Figure 12. Chromatograms Obtained for EDTA Using Varian 4100 HPLC

APPENDIX
LITERATURE SURVEY LISTING

GENERAL

- Amos, R., and Perry, S. G., "Liquid Chromatography--Columns or Thin Layers?", *J. of Chromatogr.*, 83, 1973, pp. 245-254.
- Barrall, E. M., II, and Johnson, J. F., "Gel Permeation Chromatography: Apparatus and Detectors," *Symposium on Gel Permeation Chromatography*, ACS Houston Meeting, February 22-27, 1970.
- Bombaugh, K. J., "A Practical Approach to Analytical Liquid Chromatography," *Amer. Lab.* 1969, July.
- Chandler, C. D., "High Pressure Liquid Chromatography Equipment," *J. Chrom. Sci.*, 11, 1973, pp. 468-475.
- Eisenbeiss, F., and Sieper, H., "The Potential Use of High-Performance Liquid Chromatography in Residue Analysis," *J. of Chromatogr.*, 83, 1973, pp. 439-446.
- Heftmann, E., "Liquid Chromatography--Past and Future," *J. Chrom. Sci.*, 11(6), 1973, pp. 295-298.
- Pilipenko, A. T., and Volkova, A. I., "Methods of Chemical Analysis," *Z. Lab.*, 39(5), 1973, pp. 513-536.
- Rohrschneider, L., "Chromatographic Characterization of Liquid Phases and Solutes for Column Selection and Identification," *J. Chrom. Sci.*, 11(3), 1973, pp. 160-166.
- Veening, H., "Recent Developments in Instrumentation for Liquid Chromatography," *J. Chem. Ed.*, 50(9), 1973, pp. A429-A445.
- Waters, J. L., "Preparative Liquid Chromatography," *J. Chrom. Sci.*, 9(7), 1971, pp. 429-431.

THEORETICAL AND PRACTICAL PARAMETERS

- Baumann, E. W., "Determination of Stability Constants of Hydrogen and Aluminum Fluorides with a Fluoride-Selective Electrode," *J. Inorg. Nucl. Chem.*, Vol. 31, 1969, pp. 3155-3162.
- Buy, T. S., and de Clerk, K., "A Semi-Empirical Expression for the First Moment in Non-Linear Chromatography," *J. Chrom. Sci.*, 10(12), 1972, pp. 722-724.

- de Clerk, K., and Buys, T. S., "The Effect of Sorption on Retention Times in Non-Linear Chromatography," *J. of Chromatogr.*, 84, 1973, pp. 1-6.
- de Clerk, K., and Buys, T. S., "Moments Analysis in Non-Linear Chromatography. I. The First Moment," *J. of Chromatogr.*, 6, 1971, pp. 193-202.
- Cooper, D. R., "Least Squares Analysis of Chrom. Tracings," *J. Chrom.*, 80, 1973, pp. 246-249.
- Deininger, G., and Halasz, I., "Measured Performance Errors and Loss of Resolution in Liquid Chromatography," *J. Chrom. Sci.*, 9(2), 1971, pp. 83-91.
- Fletcher, R., and Powell, M. J. D., "A Rapidly Convergent Descent Method for Minimization," *Computer J.*, 6, 1963, p. 163.
- Gallot, Z. Grubisic, and Benoit, H., "Comparison of Partition Coefficients Determined by Static and Dynamic Methods on Porous Glass Beads," *J. Chrom. Sci.*, 9(5), 1971, pp. 262-265.
- Gans, P., "Force-constant Computations. Part II. Some Model Calculations to Test the Fletcher-Powell Method and to Analyse the ILL-Conditioned Force-constant Refinement," *J. Chem. Soc.*, (A), 1971, p. 2017.
- Gans, P., and Vacca, A., "Application of the Davidon-Fletcher-Powell Method to the Calculation of Stability Constants," *Talanta*, Vol. 21, pp. 45-51.
- Goedert, M., and Guiochon, G., "The Effect of Random Noise on the Precision and Accuracy of the Measurements of the Peak Area and the Retention Time in Chromatography," *J. Chrom. Sci.*, 11(6), 1973, pp. 326-334.
- Grushka, E., Yepes-Baraya, M., and Cooke, W. D., "Amount of Stationary Phase-Time Normalization Chromatography," *J. Chrom. Sci.*, 9(11), 1971, pp. 653-664.
- Grushka, E., "Time Normalization in Liquid Chromatography," *J. Chrom. Sci.*, 10(10), 1972, pp. 616-621.
- Grushka, E., and Guiochon, G., "Optimizing Capacity Ratio in Time Normalization Chromatography," *J. Chrom. Sci.*, 10(11), 1972, pp. 649-654.
- Huber, J. F. K., "Criteria for The Choice of Liquid-Liquid Systems for Column Chromatography," *J. Chrom. Sci.*, 9(2), 1971, pp. 62-76.
- Keller, R. A., "Phase Selectivity in Gas and Liquid Chromatography," *J. Chrom. Sci.*, 11(2), 1973, pp. 49-59.
- Leary, J. J., Tsuge, S., and Isenhour, T. L., "Rohrschneider Constants: A Correction in the Method of Calculation," *J. Chrom.*, 82, 1973, pp. 366-369.
- Lill, S. A., "A Modified Davidon Method for Finding the Minimum of a Function, Using Difference Approximation for Derivatives," *Computer J.*, 13, 1970, p. 111; 14, 1971, p. 106.

- Majors, R. E., and MacDonald, F. R., "Practical Implications of Modern Liquid Chromatographic Column Performance," *J. of Chromatogr.*, 83, 1973, pp. 1969-1979.
- Martin, L. F., Bertoniere, N. R., and Rowland, S. P., "The Effects of Sorption and Molecular Size of Solutes Upon Elution From Polyhydroxylic Gels," *J. of Chromatogr.*, 64, 1972, pp. 263-270.
- Mir, L., "Effect of Mixing Devices on the Efficiency of Columns with Flow Maldistribution," *J. Chrom. Sci.*, 9(7), 1971, pp. 436-437.
- Morris, B. M., Mode, V. A., and Sisson, D. H., "Liquid Chromatography IV. Effects of Solvent Velocity on Separation Using Ion-Exchange Resin," *J. of Chromatogr.*, 71, 1972, pp. 389-393.
- Rony, P. R., and Funk, J. E., "Retention Time and the First Time Moment in Elution Chromatography. III. General Conclusions," *J. Chrom. Sci.*, 9(4), 1971, pp. 215-219.
- Rony, P. R., "The Extent of Separation: Time Normalization and Minimum Time Analysis in Elution Chromatography," *J. Chrom. Sci.*, 9(6), 1971, pp. 350-352.
- Sabatini, A., and Vacca, A., "A New Method for Least-squares Refinement of Stability Constants," *J. Chem. Soc. (Dalton)*, 1972, p. 1693.
- Sabatini, A., Vacca, A., and Gans, P., "Miniquad--A General Computer Programme For The Computation of Formation Constants from Potentiometric Data," *Talanta*, Vol. 21, pp. 53-77.
- Schneider, Hansjorg A. W., "pH-Dependent Elution Volume of Some Pyrroles Chromatographed on Sephadex G-15," *J. Chrom.*, 81, 1973, pp. 160-162.
- Schomburg, G., and Dielmann, G., "Identification by Means of Retention Parameters," *J. Chrom. Sci.*, 11(3), 1973, pp. 151-159.
- Scott, R. P. W., "Factors Affecting Peak Capacity in Liquid Chromatography," *J. Chrom. Sci.*, 9(8), 1971, pp. 449-457.
- Solms, D. J., Smuts, T. W., and Pretorius, Victor, "Displacement Peaks in Liquid Elution Chromatography," *J. Chrom. Sci.*, 9(10), 1971, pp. 600-603.
- Stewart, III, G. W., "A Modification of Davidon's Minimization Method to Accept Difference Approximations of Derivatives," *J. Assoc. Computing Machinery*, 14, 1967, pp. 72-83.
- Vink, H., "Resolution and Column Efficiency in Chromatography," *J. of Chromatogr.*, 69, 1972, pp. 237-242.
- Volf, J., Koubek, J., and Pasek, J., "A Contribution to the Measurement of Adsorption Isotherms by the Pulse Chromatograph Technique," *J. of Chromatogr.*, 81, 1973, pp. 9-17.

- Yamada, M., Nomura, N., and Shiho, D., "Automatic Liquid Chromatography of Organic Compounds. III. The Relationship Between The Chromatographic Behavior and The Chemical Structure of Benzene Derivatives," *J. of Chromatogr.*, 64, 1972, pp. 253-262.
- Yoshino, T., Murakami, S., Kagawa, M., and Araragi, T., "Formation Constants of Zinc(II) Complexes with Semi-Xylenol Orange," *Talanta*, Vol. 21, pp. 79-85.

STATIONARY PHASE

- Asshauer, J., and Halasz, I., "Reproducibility and Efficiency of Columns Packed with 10 μ Silica in Liquid Chromatography," *J. Chrom. Sci.*, 12, 1974, pp. 139-147.
- Done, J. N., and Knox, J. H., "The Performance of Packings in High Speed Liquid Chromatography II. ZIPAX The Effect of Particle Size," *J. Chrom. Sci.*, 10(10), 1972, pp. 606-612.
- Freeman, D. H., "The Gels for Liquid Chromatography," *J. Chrom. Sci.*, 11(4), 1973, pp. 175-180.
- Frolov, I. I., Vorobyoeva, R. G., Mironova, I. V., Chernov, A. Z., and Yashin, Y. I., "Silochroms as Adsorbents and Supports in Liquid Chromatography," *J. of Chromatogr.*, 80, 1973, pp. 167-171.
- Grant, D. W., "The Use of Gel-Coated Glass Microspherical Supports for Improved Column Performance and the Rapid Separation of Isomeric Compounds," *J. of Chromatogr.*, 81, 1973, pp. 33-45.
- Kennedy, G. J., and Knox, J. H., "The Performance of Packings in High Performance Liquid Chromatography (HPLC) I. Porous and Surface Layered Supports," *J. Chrom. Sci.*, 10(9), 1972, pp. 549-556.
- Kirkland, J. J., "High-Performance Liquid Chromatography with Porous Silica Microspheres," *J. Chrom. Sci.*, 10(10), 1972, pp. 593-599.
- "High Speed Liquid-Partition Chromatography with Chemically Bonded Organic Stationary Phases."
- Kirkland, J. J., "Porous Silica Microsphere Column Packings for High-Speed Liquid-Solid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 149-167.
- Knox, J. H., and Vasvari, G., "The Performance of Packings in High-Speed Liquid Chromatography. III. Chemically Bonded Pellicular Materials," *J. of Chromatogr.*, 83, 1973, pp. 181-194.
- Leitch, R. E., and DeStefano, J. J., "Column Packings for Modern Liquid Chromatography," *J. Chrom. Sci.*, 11(3), 1973, pp. 105-113.
- Locke, D. C., "Chemically Bonded Stationary Phases for Liquid Chromatography," *J. Chrom. Sci.*, 11(3), 1973, pp. 120-128.

- Lynn, T. R., "High Resolution-Low Pressure Liquid Chromatography," *J. Chrom. Sci.*, 12, 1974, pp. 76-79.
- Majors, R. E., "Effect of Particle Size on Column Efficiency in Liquid-Solid Chromatography," *J. Chrom. Sci.*, 11(2), 1973, pp. 88-95.
- Mattox, V. R., Goodrich, J. E., and Litwiller, R. D., "Liquid Ion Exchangers for Chromatography of Steroidal Glucosiduronic Acids and Other Polar Compounds," *J. of Chromatogr.*, 66, 1972, pp. 337-346.
- Mikes, F., Schurig, V., and Gil-Av, E., "Complex-Forming Stationary Phases in High-Speed Liquid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 91-97.
- Popl, M., Dolansky, V., and Mostecky, J., "Adsorption Elution Chromatography of Nitrogen-Containing Heterocycles on Alumina," *J. of Chromatogr.*, 74, 1972, pp. 51-57.
- Ray, S., and Frei, R. W., "Separation of Polynuclear Aza-Heterocyclics by High-Speed Liquid Chromatography on a Chemically Bonded Stationary Phase," *J. of Chromatogr.*, 71, 1972, pp. 451-457.
- Unger, K., and Schick-Kalb, J., "Preparation of Porous Silica Spheres for Column Liquid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 5-9.

EXPERIMENTAL ELUTION

- Aitzetmüller, K., "A Multi-Component Preparative Liq.-Chrom. System," *J. Chrom.*, 73, 1972, pp. 248-252.
- Baker, D. R., Henry, R. A., Williams, R. C., and Hudson, D. R., "Preparative Columns in High-Speed Liquid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 233-243.
- Deininger, G., and Halasz, I., "Control of Flow Rate in High Pressure Liquid Chromatography," *J. of Chromatogr.*, 60, 1971, pp. 65-73.
- DeStefano, J. J., and Beachell, H. C., "Performance of Larger Diameter Columns for High-Speed Liquid-Solid Chromatography," *J. Chrom. Sci.*, 10(11), 1972, pp. 654-662.
- Felton, H., "Performance of Components of a High Pressure Liquid Chromatography System," *J. Chrom. Sci.*, 7(1), 1969, pp. 13-16.
- Henry, R. A., Byrne, S. H., and Hudson, D. R., "High Speed Recycle Chromatography Using an Alternate Pumping Principle," *J. Chrom. Sci.*, 12, 1974, pp. 197-199.
- Huber, J. F. K., and Van Der Linden, R., "Column Switching in High-Pressure Liquid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 267-277.

Krejci, M., and Vespalec, R., "Sampling System and Analysis of Basic Components of Sprays by Liquid Chromatography," *J. of Chromatogr.*, 65, 1972, pp. 333-340.

"Precise Quantitative Analysis with a Stable, High-Speed Liquid-Liquid Chromatography Column," *J. Chrom. Sci.*, 9(9), 1971, pp. 531-535.

Scott, C. D., and Pitt, Jr., W. W., "Differential Chromatography Using Dual, Coupled Parallel Columns," *J. Chrom. Sci.*, 10(12), 1972, pp. 740-743.

Scott, R. P. W., and Kucera, P., "The Design of Column Connection Tubes for Liquid Chromatography," *J. Chrom. Sci.*, 9(11), 1971, pp. 641-644.

Thurman, R. G., and Burke, M. F., "A Simple On-Line Flow Sensor for Gas Chromatography," *J. Chrom. Sci.*, 9(3), 1971, pp. 181-183.

Vigh, G., "A Simple, Noise-Free, Starting-Point Generating Device for Liq.-Chrom.," *J. Chrom.*, 74, 1972, p. 128.

GRADIENT ELUTION

Byrne, S. H., Schmit, J. A., and Johnson, P. E., "A Multifunctional Gradient Device for Use in High-Speed Liquid Chromatography," *J. Chrom. Sci.*, 9(10), 1971, pp. 592-595.

"An Automated Simplified Eluent Gradient-Generating System for Use in Liquid Chromatography," *J. of Chromatogr.*, 75, 1973, pp. 175-186.

Scott, R. P. W., "Gradient Elution Facilities for LC Using the Continuous and Incremental Methods of Solvent Mixing," *J. Chrom. Sci.*, 9(7), 1971, pp. 385-389.

Scott, R. P. W., and Kucera, P., "An Apparatus for Use With Incremental Gradient Elution," *J. Chrom. Sci.*, 11(2), 1973, pp. 83-87.

Scott, R. P. W., and Kucera, P., "Incremental Gradient Elution. Some Factors that Affect Resolution and Analysis Time," *J. of Chromatogr.*, 83, 1973, pp. 257-266.

DETECTORS

Bakken, M., and Stenberg, V. I., "The Interferometer as a Detector for Liquid Chromatography," *J. Chrom. Sci.*, 9, 1971, pp. 603-607.

Bylina, A., Sybilska, D., Frabowski, Z. R., and Koszewski, J., "Rapid-Scanning Spectrophotometry as a New Detection System in Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 357-362.

- Cassidy, R. M., and Frei, R. W., "A Fluorescence Detector for High-Speed Chromatography," *J. of Chromatogr.*, 72, 1972, pp. 293-301.
- Cavina, G., Moretti, G., Mollica, A., and Antonini, R., "Analysis of Steroid Mixtures by Column Chromatography with Continuous Monitoring of the Eluate by a Flame Ionisation Detector," *J. of Chromatogr.*, 60, 1971, pp. 179-184.
- Conlon, R. D., "Liquid Chromatography Detectors," *Anal. Chem.*, 41(4), 1969, pp. 107A-115A.
- Deininger, G., and Halasz, I., "Modification of a Differential-Refractometer-Detector for Liquid Chromatography," *J. Chrom. Sci.*, 8(9), 1970, pp. 499-501.
- DeLew, R. B., "Improvements in the Performance of the Thermal Conductivity Detector," *J. Chrom. Sci.*, 10, 1972, pp. 60-605.
- Dubsky, H., "A Disc Detector for Liquid Chromatography," *J. of Chromatogr.*, 71, 1972, pp. 395-403.
- Ford, A., and Meloan, C. E., "An Inexpensive Conductivity Monitor for Column Operation," *J. Chem. Ed.*, 50(1), 1973, pp. 85-86.
- Frei, R. W., and Lawrence, J. F., "Fluorogenic Labelling in High-Speed Liquid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 321-330.
- Gerding, J. J. T., Kemper, H. J. M., Lamers, B. J. M., and Gerding, M. H., "A New Highly Sensitive Detection System for Peptides and Proteins in Column Effluents," *J. Chrom.*, 66, 1972, pp. 145-152.
- Hatano, H., and Yamamoto, Y., "A High-Speed Liquid Chromatograph with a Flow-Spectrofluorimetric Detector and the Ultramicro-Determination of Aromatic Compounds," *J. of Chromatogr.*, 83, 1973, pp. 373-380.
- Janghorbani, M., and Freund, H., "Application of a Piezoelectric Quartz Crystal as a Partition Detector. Development of a Digital Sensor," *Anal. Chem.*, 45(2), 1973, pp. 325-332.
- Johnson, D. C., and Larochelle, J., "Forced-Flow Liquid Chromatography with a Coulometric Detector," *Talanta*, Vol. 20, pp. 959-971.
- Karasek, F. W., and Gibbins, K. R., "A Gas Chromatograph Based on the Piezoelectric Detector," *J. Chrom. Sci.*, 9(9), 1971, pp. 535-540.
- Katz, S., and Thacker, L. H., "A New Sensitive Ultraviolet Detection System for Carbohydrates Eluted During Column Chromatography," *J. of Chromatogr.*, 64, 1972, pp. 247-252.
- Keller, R. A., "Principles of Detection," *J. Chrom. Sci.*, 11(5), 1973, pp. 223-226.
- Krejci, M., and Pospisilova, N., "Experimental Comparison of Some Detectors Used in High-Efficiency Liquid Chromatography," *J. of Chromatogr.*, 73, 1972, pp. 105-115.

- Lapidus, R. M., and Karmen, A., "An Efficient Flame Ionization Detection System for Liquid Chromatography," *J. Chrom. Sci.*, 10, 1972, pp. 103-106.
- Munk, M. N., "Comparison of Low Dead Volume UV Absorption, Refractive Index, and Heat of Adsorption Detectors for Liquid Chromatography," *J. Chrom. Sci.*, 8(9), 1970, pp. 491-496.
- Nota, G., and Palombari, R., "Use of an Electron Capture Detector for Monitoring in Liquid Chrom.,", *J. Chrom.*, 62, 1971, pp. 153-155.
- Pellizzari, E. D., and Sparacino, C. M., "Scanning Fluorescence Spectrometry Combined with Ultraviolet Detection of High Pressure Liquid Chromatographic Effluents," *Anal. Chem.*, 45(2), 1973, pp. 378-381.
- Polesuk, J., "Chromatographic Detection," *J. Chrom. Sci.*, 11(5), 1973, pp. 226-233.
- Poppe, H., and Kuyster, J., "Construction of a Permittivity Detector for Liquid Chromatography," *J. Chrom. Sci.*, 10, 1972, pp. 16A-18A.
- Pretorius, V., and van Rensburg, J. F. J., "Improvements to the Wire Solute Transport Detector for Liquid Chromatography: Coated Wires," *J. Chrom. Sci.*, 11, 1973, pp. 355-357.
- Prydz, S., Meto, T. B., Koren, J. F., and Eriksen, E. L., "Fast Radiochromatographic Detection of Tritium with 'Liquid' Scintillators at Low Temperatures," *Anal. Chem.*, 42(2), 1970, pp. 156-161.
- Roth, M., and Hampai, A., "Column Chromatography of Amino Acids with Fluorescence Detection," *J. of Chromatogr.*, 83, 1973, pp. 353-356.
- Schulten, H. R., and Beckey, H. D., "Potentiality of the Coupling of Column Liquid Chromatography and Field Desorption Mass Spectrometry," *J. of Chromatogr.*, 83, 1973, pp. 315-320.
- Schulz, W. W., and King, Jr., W. H., "A Universal Mass Detector for Liquid Chromatography," *J. Chrom. Sci.*, 11, 1973, pp. 343-348.
- Schutte, L., "Continuous Detection of Radioactive Effluents in Liquid Chromatography by Heterogeneous or Homogeneous Scintillation Counting," *J. Chromatogr.*, 72, 1972, pp. 303-309.
- Scott, R. P. W., "A Theoretical Treatment of the Heat of Adsorption Detector," *J. Chrom. Sci.*, 11, 1973, pp. 349-353.
- Stolyhwo, A., Privett, O. S., and Erdahl, W. L., "An Improved Flame Ionization Detector and Associated Transport System for Liquid Chromatography," *J. Chrom. Sci.*, 11(5), 1973, pp. 263-267.
- Thacker, L. H., "A Miniature Flow Fluorometer for Liquid Chromatography," *J. of Chromatogr.*, 73, 1972, pp. 117-123.
- Thacker, L. H., Pitt, Jr., W. W., Katz, S., and Scott, C. D., "Miniature Photometers for Liquid Chromatography," *Clin. Chem.*, 16(8), 1970, pp. 626-632.

- Thacker, L. H., Scott, C. D., and Pitt, Jr., W. W., "A Miniaturized Ultra-violet Flow Photometer for Use in Liquid Chromatographic Systems," *J. of Chromatogr.*, 51, 1970, pp. 175-181.
- Veening, H., "Liquid Chromatography Detectors--Part One," *J. Chem. Ed.*, 47(9), 1970, pp. A549-A568.
- Veening, H., "Liquid Chromatography Detectors--Part Two," *J. Chem. Ed.*, 47(10), 1970, pp. A675-A686.
- Vespalec, R., and Hana, K., "Performance of the Capacitance Detector for Liquid Chromatography," *J. of Chromatogr.*, 65, 1972, pp. 53-69.

APPLICATION

- Aitzetmüller, K., "Frontal Elution Liq. Chrom. of a 'Total Artifacts' Peak in Frying Oils," *J. Chrom.*, 79, 1973, pp. 329-334.
- Aitzetmüller, K., "Investigation of Heated and Oxidized Oils and Fats by Gradient Elution Liquid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 461-469.
- Baczuk, R. J., Landram, G. K., Dubois, R. J., and Dehm, H. C., "Liquid Chromatographic Resolution of Racemic β -3,4-Dihydroxyphenylalanine," *J. of Chromatogr.*, 60, 1971, pp. 351-361.
- Bailey, F., and Brittain, P. N., "High-Efficiency Liquid Chromatography in Pharmaceutical Analysis," *J. of Chromatogr.*, 83, 1973, pp. 431-437.
- Bengtsson, L., and Samuelson, O., "Anion-Exchange Chromatography of Dicarboxylic Acids in Sulphate Medium," *J. of Chromatogr.*, 61, 1971, pp. 101-109.
- Carey, M. A., and Persinger, H. E., "Liquid Chromatographic Determination of Traces of Aliphatic Carbonyl Compounds and Glycols as Derivatives that Contain the Dinitrophenyl Group," *J. Chrom. Sci.*, 10(9), 1972, pp. 537-543.
- Cashman, P. J., Thornton, J. I., and Shelman, D. L., "High Pressure Liquid Chromatographic Separation of Phenethylamines of Forensic Interest," *J. Chrom. Sci.*, 11(1), 1973, pp. 7-9.
- Cassidy, R. M., LeGay, D. S., and Frei, R. W., "Analysis of Phenols by Derivatization and High-Speed Liquid Chromatography," *J. Chromatogr. Sci.*, 12, 1974, pp. 85-89.
- Cavina, G., Moretti, G., and Cantafora, A., "Analysis of Corticosteroids in Mixtures by Gradient Elution Liquid Chromatography," *J. of Chromatogr.*, 80, 1973, pp. 89-100.
- Coali, J. O., and Juhasz, A. A., "Application of High Speed Liquid Chromatography to the Qualitative Analysis of Compounds of Propellant and Explosives Interest," *J. Chromatogr. Sci.*, 12, 1974, pp. 51-56.

- Cox, G. B., "Estimation of Volatile N-Nitrosamines by High-Performance Liquid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 471-481.
- Davankov, V. A., and Rogozhin, S. V., "Ligand Chromatography as a Novel Method for the Investigation of Mixed Complexes: Stereoselective Effects in α -Amino Acid Copper(II) Complexes," *J. Chrom.*, 60, 1971, pp. 280-283.
- Davankov, V. A., Rogozhin, S. V., Semechkin, A. V., and Sukhova, T. P., "Ligand-Exchange Chromatography of Racemates. Influence of the Degree of Saturation of the Asymmetric Resin by Metal Ions on Ligand Exchange," *J. of Chromatogr.*, 82, 1973, pp. 359-365.
- Dennison, C., "Sodium Chloride in Buffers for Amino Acid Analysis Application to the Analysis of Lysine in Maize Samples," *J. Chromatogr.*, 89, 1974, pp. 84-86.
- Deyl, Z., "Column Chromatographic Separation of Dansyl Amino Acids," *J. of Chromatogr.*, 69, 1972, pp. 129-133.
- Dolphin, R. J., "The Analysis of Estrogenic Steroids in Urine by High-speed Liquid Chromatography," *J. of Chromatogr.*, 83, 1973, pp. 421-429.
- Floridi, A., "An Improved Method for the Automated Analysis of Sugars by Ion-Exchange Chromatography," *J. of Chromatogr.*, 59, 1971, pp. 61-70.
- Frei, R. W., Lawrence, J. F., Hope, J., and Cassidy, R. M., "Analysis of Carbamate Insecticides by Fluorogenic Labelling and High-Speed Liquid Chromatography," *J. Chromatogr. Sci.*, 12, 1974, pp. 40-44.
- Funasaka, W., Hanai, T., Fujimura, K., and Ando, T., "Non-aqueous Solvent Chromatography. II. Separation of Benzene Derivatives in the Anion-Exchange and n-Butyl Alcohol System," *J. Chrom.*, 72, 1972, pp. 187-191.
- Gabriel, T. F., and Michalewsky, J., "Analysis of DNA Derivatives II. High-Pressure Liquid Anion-Exchange Chromatography of Deoxyribonucleotides," *J. of Chromatogr.*, 67, 1972, pp. 309-314.
- Ghosh, A., Hogue, M., and Dutta, J., "Separation of Polyunsaturated Fatty Acid Esters by Argentation Column Chromatography on Silicic Acid," *J. Chrom.*, 69, 1972, pp. 207-208.
- Goldie, A. H., and Subden, R. E., "Separation of the Neutral Carotenoids of *Neurospora Crassa* Using Concave Gradient Elution Chrom.," *J. Chrom.*, 84, 1973, pp. 192-194.
- Heacock, R. A., Langille, K. R., MacNeil, J. D., and Frei, R. W., "A Preliminary Investigation of the High-Speed Liq. Chrom. of Some Ergot Alkaloids," *J. Chrom.*, 77, 1973, pp. 425-430.
- Henry, R. A., Schmit, J. A., and Dieckman, J. F., "The Analysis of Steroids and Derivatized Steroids by High Speed Liquid Chromatography," *J. Chrom. Sci.*, 9(9), 1971, pp. 513-520.

- Hindley, A. H., "The Determination of the Unsulphated Material Contents of Sulphated Surface-Active Agents by Liquid Chromatography," *J. of Chromatogr.*, 67, 1972, pp. 149-152.
- Horwitz, E. P., and Bloomquist, C. A. A., "High-Speed Radiochemical Separations by Liquid-Liquid Chromatography Using a CSP Support. I. Performance of Quaternary Ammonium Chloride-Zipax System for the Elution of Cd(II) with HCl," *J. Chromatogr. Sci.*, 12, 1974, pp. 11-22.
- Inaba, T., and Brien, J. F., "Determination of the Major Urinary Metabolite of Diphenylhydantoin by High-Performance Liquid Chromatography," *J. of Chromatogr.*, 80, 1973, pp. 165-171.
- Jane, I., and Wheals, B. B., "The Characterization of LSD in Illicit Preparations by Pressure-Assisted Liq. Chrom. and Gas Chrom.," *J. Chrom.*, 84, 1973, pp. 181-186.
- Jolliffe, G. H., and Shellard, E. J., "Separation of Some Oxindole Alkaloids using High-Speed LC.," *J. Chrom.*, 81, 1973, pp. 150-151.
- Krol, G. J., Mannan, C. A., Gemmill, Jr., F. Q., Hicks, G. E., and KHO, B. T., "High-Efficiency Liquid Chromatographic Separation of Vitamin D from Precaiferol," *J. of Chromatogr.*, 74, 1972, pp. 43-49.
- Kunzru, D., and Frei, R. W., "Separation of Aromatic Amine Isomers by High-Pressure Liquid Chromatography on Cadmium-Impregnated Silica Gel Columns," *J. Chromatogr. Sci.*, 12, 1974, pp. 191-196.
- Lawrence, J. G., "High-Speed Liquid Chromatography of Non-Polar Lipids," *J. of Chromatogr.*, 84, 1973, pp. 299-308.
- Lindqvist, B., Sjogren, I., and Nordin, R., "Preparative Fractionation of Tri-glyceride Mixtures According to Acyl Carbon Number, Using Hydroxylalkoxypropyl Sephadex," *J. Lipid Res.*, 15, 1974, pp. 65-73.
- Lkimisch, H. J., "Separation of Polycyclic Aromatic Hydrocarbons by High-Pressure Liquid Chromatography. Selective Separation System for the Quantitative Determination of Isomeric Benzpyrenes and of Coronene," *J. of Chromatogr.*, 83, 1973, pp. 11-14.
- Mousaebois, C., Flimal, J., and Osinski, P., "The Spectra of N- α -trifluoroacetyl-DL-lysine from Potassium Trifluoroacetate by Liq.-Chrom.," *J. Chrom.*, 68, 1972, pp. 262-263.
- Nelson, J. J., "Quantitation of Sodium Saccharin, Sodium Benzoate and Other Food Additives by High Speed Liquid Chromatography," *J. Chrom. Sci.*, 11(1), 1973, pp. 28-35.
- Nelson, D. J., Bugge, C. J. L., Krasny, H. C., and Zimmerman, T. P., "Separation of 6-Thiopurine Derivatives on Deae-Sephadex Columns and in the High-pressure Liquid Chromatograph," *J. of Chromatogr.*, 77, 1973, pp. 181-190.
- Papa, L. J., and Turner, L. P., "Chromatographic Determination of Carbonyl Compounds as Their 2,4-Dinitrophenylhydrazones II. High Pressure Liquid Chromatography," *J. Chrom. Sci.*, 10(12), 1972, pp. 747-750.

- Pfadenhauer, E. H., "Rapid Determination of Some Plasma Oxypurines Using High-Pressure Liquid Chromatography," *J. of Chromatogr.*, 81, 1973, pp. 85-92.
- Pickett, J. A., "Use of Micro-Bead Anion-Exchange Resin for Direct Estimation of Flavour Nucleotides in Complex Solutions," *J. Chrom.*, 81, 1973, pp. 156-159.
- Pound, N. J., McGilveray, I. J., and Sears, R. W., "Analysis of Phenylbutazone in Plasma by High-Speed Liquid Chromatography," *J. of Chromatogr.*, 89, 1974, pp. 23-30.
- Ramsden, D. B., and Louis, L. N., "Use of Simple Concentration Gradients for the Fractionation of Human Serum Proteins on Deae-Cellulose, with Especial Reference to the Isolation of Albumin, Prealbumin, Haemopexin and Transferrin," *J. of Chromatogr.*, 84, 1973, pp. 87-94.
- Rao, G. H. R., and Anders, M. W., "Aflatoxin Detection by High-Speed Liq. Chrom. and Mass Spectrometry," *J. Chrom.*, 84, 1973, pp. 402-406.
- Rouser, G., "Quantitative Liquid Column and Thin Layer Chromatography of Lipids and Other Water Insoluble Substances, Elution Selectivity Principles, and a Graphic Method for Pattern Analysis of Chromatographic Data," *J. Chrom. Sci.*, 11(2), 1973, pp. 60-76.
- Schmit, J. A., Henry, R. A., Williams, R. C., and Dieckman, J. F., "Applications of High Speed Reversed-Phase Liquid Chromatography," *J. Chrom. Sci.*, 9(11), 1971, pp. 645-651.
- Scott, C. D., Chilcote, D. D., Katz, S., and Pitt, Jr., W. W., "Advances in the Application of High Resolution Liquid Chromatography to the Separation of Complex Biological Mixtures," *J. Chrom. Sci.*, 11, 1973, pp. 96-100.
- Sisson, D. H., and Mode, V. Alan, "High-Speed Separation of the Rare Earths by Ion Exchange: Part II," *J. of Chromatogr.*, 66, 1972, pp. 129-135.
- Sparatorico, A. L., and Coulter, B., "Evaluation of the Efficiency of Polymer Fractionation by the Column Elution Method," *J. of Chromatogr.*, 79, 1973, pp. 121-128.
- Stahl, K. W., Schlimme, E., and Bojanowski, D., "High-Pressure Liquid Chromatography of Modified Purine Mononucleotides and Nucleosides," *J. of Chromatogr.*, 83, 1973, pp. 395-404.
- Stevenson, R. L., and Burtis, C. A., "The Analysis of Aspirin and Related Compounds by Liquid Chromatography," *J. of Chromatogr.*, 61, 1971, pp. 253-261.
- Stolyhwo, A., and Privett, O. S., "Studies on the Analysis of Lipid Classes by Gradient Elution Absorption Chromatography," *J. Chrom. Sci.*, 11(1), 1972, pp. 20-25.
- Touchstone, J. C., and Wortmann, W., "High-Pressure Liq. Chrom. of Corticosteroids," *J. Chrom.*, 76, 1973, pp. 244-247.

- Van de Weerdhof, T., Wiersum, M. L., and Reissenweber, H., "Application of Liquid Chromatography in Food Analysis," *J. of Chromatogr.*, 83, 1973, pp. 455-460.
- Vaughan, C. G., Wheals, B. B., and Whitehouse, M. J., "The Use of Pressure-Assisted Liquid Chromatography in the Separation of Polynuclear Hydrocarbons," *J. of Chromatogr.*, 78, 1973, pp. 203-210.
- Vecchi, M., Vesely, J., and Oesterhelt, G., "Applications of High-Pressure Liquid Chromatography and Gas Chromatography to Problems in Vitamin A Analysis," *J. of Chromatogr.*, 83, 1973, pp. 447-453.
- Williams, R. C., Schmit, J. A., and Henry, R. A., "Quantitative Analysis of the Fat Soluble Vitamins by High-Speed Liquid Chromatography," *J. Chrom. Sci.*, 10(8), 1972, pp. 494-501.
- Wittwer, Jr., J. D., and Kluckhohn, J. H., "Liquid Chromatographic Analysis of LSD," *J. Chrom. Sci.*, 11(1), 1973, pp. 1-3.
- Wortmann, W., Schnabel, C., and Touchstone, J. C., "Quantitative Determination of Corticosteroids from Plasma by High-Pressure Liq. Chrom.," *J. Chrom.*, 84, 1973, pp. 396-401.
- Zitko, V., "Chromatography of Chlorinated Paraffins on Alumina and Silica Columns," *J. Chrom.*, 81, 1973, pp. 152-155.

AUTOMATED DEVICES

- Ascione, P. P., Zagar, J. B., and Chrekian, G. P., "An Automated Liquid Chromatographic Method for the Determination of Tetracycline Antibiotics," *J. of Chromatogr.*, 65, 1972, pp. 377-386.
- Barth, H., Dallmeier, E., Courtois, G., Keller, H. E., and Karger, B. L., "A Study of Precision in Modern Liquid Chromatography Using a Dedicated Computer," *J. of Chromatogr.*, 83, 1973, pp. 289-311.
- Bonnelyeke, B. E., "Computer-Generated Chromatograms," *J. Chrom.*, 61, 1971, pp. 322-324.
- Buchanan, J. E., and Maher, T. P., "Computer-Drawn Histograms as 'Fingerprints' of Complex G. C. Fractions," *J. Chrom. Sci.*, 9, 1971.
- Davies, B. H., and Mercer, E. I., "The Liquid Spectroradiochromatograph--An Automated Method for the Simultaneous Separation, Identification, Purification, Estimation and Radioassay of the Components of a Mixture of Unsaponifiable Lipids," *J. of Chromatogr.*, 46, 1970, pp. 161-172.
- Elkin, K., Pierrou, L., Ahlborg, U. G., Holmstedt, B., and Lindgren, J. E., "Computer-Controlled Mass Fragmentography with Digital Signal Processing," *J. of Chromatogr.*, 81, 1973, pp. 47-55.

- Fox, M. A., "Programs for Use with the Automatic Amino Acid Analyser to Identify, Compute and Correlate Amino Acid Concentrations in Biological Samples," *J. of Chromatogr.*, 89, 1974, pp. 61-72.
- Frazer, J. T., and Guran, B. T., "Use of a Magnetic Tape Cassette Recorder with an On-Line GC Data System," *J. Chromatogr. Sci.*, 9, 1971, pp. 718-721.
- Gill, J. M., and Deans, D. R., "Symposium on Chromatography and Computers ... an Economical Approach for Every Laboratory," *J. Chrom. Sci.*, 9(12), 1971, p. 705.
- Hegedus, L. L., and Petersen, E. E., "Integration of Chromatographic Signals by Digital Computers: an Approach for the Small Chromatographic Laboratory where Digital Computer Services are Available," *J. Chrom. Sci.*, 9(9), 1971, pp. 551-553.
- Hettinger, J. D., Hubbard, J. R., Gill, J. M., and Miller, L. A., "A New Computing Integrator for Chromatography," *J. Chromatogr. Sci.*, 9, 1971, pp. 710-717.
- Hunter, I. R., and Walden, M. K., "A Simple Leak Detector for the Continuous Monitoring of Septum Leaks," *J. Chrom. Sci.*, 10(12), 1972, p. 751.
- Jackson, H. W., "Gas Chromatography Automation by Integrator and Time Share," *J. Chrom. Sci.*, 9(12), 1971, pp. 706-709.
- Longbottom, J. E., "The Use of a Programmable Calculator with Plotting Capabilities to Assist in Gas Chromatographic Computations," *J. Chrom. Sci.*, 11(1), 1973, pp. 13-16.
- Marsden, N. V. B., Oberg, P. A., and Persson, A., "A Paper Tape Reading Control System for Programming Sample Collection Intervals in Column Chromatography," *J. Chrom.*, 69, 1972, pp. 385-387.
- Oppergaard, A., "The Use of Septum/Syringe/Injector in Gas Chromatography. Problems and Improvements," *J. Chrom. Sci.*, 10(12), 1972, pp. 716-721.
- Schnipelsky, P., Solsky, J. F., and Grushka, E., "An Automatic Sequencer for Chromatographic Injections and Controls," *J. Chrom. Sci.*, 12, 1973, pp. 45-49.
- Schomburg, G., Weeke, F., Weimann, B., and Ziegler, E., "Chromatography On-Line to the Mülheim Computer System," *J. Chrom. Sci.*, 9, 1971, pp. 735-741.
- Scott, R. M., "The Use of the Computer in Teaching the Theory of Chromatography," *J. of Chromatogr.*, 60, 1971, pp. 313-318.
- Seim, T. O., and Prydz, S., "Computerized Contour Mapping Applied to Two-Dimensional Radiochromatograms," *J. of Chromatogr.*, 73, 1972, pp. 183-192.
- Smuts, T. W., Richter, P. W., and Pretorius, V., "An Investigation of the Response of the Micro-Adsorption Detector by Computer Simulation," *J. Chrom. Sci.*, 9(8), 1971, pp. 457-462.

Thurman, R. G., Mueller, D. A., and Burke, M. F., "Real-Time Computer Control of A Gas Chromatograph," *J. Chrom. Sci.*, 9(2), 1971, pp. 77-83.

Winfrey, J. C., and Bethel, Jr., C. E., "The Use of Programmable Electronic Calculators to Process GC Data," *J. Chrom. Sci.*, 9(6), 1971, pp. 353-355.